

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020148.D
 Acq On : 22 Jan 2021 20:10
 Operator : SY/MD
 Sample : M1181-15DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E34DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	84	rVB2	301035	310629	12.78%	1.863%
2	1.570	142	149	161	rVB	220873	245211	10.09%	1.471%
3	2.110	307	317	343	rVB	381201	572698	23.57%	3.435%
4	2.708	499	503	507	rVB4	755	611	0.03%	0.004%
5	2.724	507	508	510	rBV	652	312	0.01%	0.002%
6	2.769	511	522	537	rVB5	8511	16625	0.68%	0.100%
7	2.865	549	552	556	rBV3	476	395	0.02%	0.002%
8	3.000	591	594	597	rBV4	747	479	0.02%	0.003%
9	3.049	597	609	624	rVV8	5427	12335	0.51%	0.074%
10	3.103	624	626	629	rBV	468	254	0.01%	0.002%
11	3.180	647	650	652	rBV	475	345	0.01%	0.002%
12	3.209	657	659	662	rBV	343	210	0.01%	0.001%
13	3.274	674	679	680	rBV	494	319	0.01%	0.002%
14	3.322	692	694	695	rBV	824	293	0.01%	0.002%
15	3.463	734	738	740	rBV4	495	478	0.02%	0.003%
16	3.486	743	745	749	rBV2	357	193	0.01%	0.001%
17	3.598	776	780	782	rBV4	425	383	0.02%	0.002%
18	3.650	792	796	797	rBV	570	340	0.01%	0.002%
19	3.676	802	804	807	rBV3	418	311	0.01%	0.002%
20	3.746	817	826	827	rBV6	1009	1336	0.05%	0.008%
21	3.840	851	855	859	rBV4	668	661	0.03%	0.004%
22	3.914	859	878	913	rBV2	918149	2430033	100.00%	14.576%
23	4.354	1000	1015	1040	rBV	292518	704829	29.00%	4.228%
24	4.582	1085	1086	1087	rBV	521	189	0.01%	0.001%
25	4.749	1136	1138	1139	rBV	395	149	0.01%	0.001%
26	4.872	1173	1176	1179	rBV3	582	344	0.01%	0.002%
27	4.901	1184	1185	1188	rVB2	366	144	0.01%	0.001%
28	4.920	1188	1191	1192	rBV	720	328	0.01%	0.002%
29	4.952	1199	1201	1203	rBV2	587	263	0.01%	0.002%
30	4.971	1204	1207	1209	rBV3	474	269	0.01%	0.002%
31	5.052	1213	1232	1265	rBV2	735256	1868065	76.87%	11.205%
32	5.505	1369	1373	1382	rVB6	901	1107	0.05%	0.007%
33	5.537	1382	1383	1385	rBV	573	191	0.01%	0.001%
34	5.550	1385	1387	1389	rVB	537	215	0.01%	0.001%
35	5.621	1397	1409	1436	rBV	552284	1098821	45.22%	6.591%
36	5.920	1487	1502	1529	rBV2	185699	395183	16.26%	2.370%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012221\
 Data File : VW020148.D
 Acq On : 22 Jan 2021 20:10
 Operator : SY/MD
 Sample : M1181-15DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E34DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.074	1536	1550	1577	rBV	415626	842313	34.66%	5.052%
38	6.261	1606	1608	1611	rBV2	492	348	0.01%	0.002%
39	6.376	1642	1644	1649	rVB3	336	213	0.01%	0.001%
40	6.399	1649	1651	1652	rBV	277	124	0.01%	0.001%
41	6.553	1696	1699	1702	rBV	207	128	0.01%	0.001%
42	6.579	1704	1707	1711	rVB2	246	158	0.01%	0.001%
43	6.624	1714	1721	1722	rBV2	415	462	0.02%	0.003%
44	6.650	1727	1729	1734	rBV4	560	425	0.02%	0.003%
45	6.878	1798	1800	1802	rBV2	418	196	0.01%	0.001%
46	6.926	1810	1815	1817	rBV4	611	619	0.03%	0.004%
47	6.991	1822	1835	1862	rBV	221739	405291	16.68%	2.431%
48	7.322	1925	1938	1957	rBV	846068	1472224	60.58%	8.831%
49	7.627	2023	2033	2059	rBV	153246	266824	10.98%	1.600%
50	7.782	2079	2081	2084	rBV3	538	279	0.01%	0.002%
51	7.981	2132	2143	2159	rBV	186143	311304	12.81%	1.867%
52	8.093	2168	2178	2211	rBV2	438122	854886	35.18%	5.128%
53	8.454	2288	2290	2294	rBV	347	228	0.01%	0.001%
54	8.675	2356	2359	2365	rVB3	1135	1065	0.04%	0.006%
55	8.720	2369	2373	2375	rBV3	684	523	0.02%	0.003%
56	8.762	2384	2386	2388	rBV	405	159	0.01%	0.001%
57	8.855	2404	2415	2450	rBV	829346	1352989	55.68%	8.116%
58	9.010	2460	2463	2465	rBV3	549	392	0.02%	0.002%
59	9.216	2523	2527	2529	rBV	979	837	0.03%	0.005%
60	9.254	2538	2539	2542	rBV2	279	146	0.01%	0.001%
61	9.312	2553	2557	2558	rVV2	291	193	0.01%	0.001%
62	9.322	2558	2560	2565	rVV	418	324	0.01%	0.002%
63	9.344	2565	2567	2571	rVV	388	241	0.01%	0.001%
64	9.363	2571	2573	2576	rVV	217	129	0.01%	0.001%
65	9.405	2584	2586	2589	rBV	193	105	0.00%	0.001%
66	9.515	2618	2620	2625	rBV3	382	287	0.01%	0.002%
67	9.537	2625	2627	2628	rBV3	211	91	0.00%	0.001%
68	9.585	2638	2642	2645	rBV3	303	306	0.01%	0.002%
69	9.627	2653	2655	2657	rBV	222	95	0.00%	0.001%
70	9.804	2708	2710	2711	rBV	239	91	0.00%	0.001%
71	9.987	2765	2767	2770	rVB3	419	192	0.01%	0.001%
72	10.032	2778	2781	2783	rBV2	354	211	0.01%	0.001%
73	10.052	2783	2787	2788	rBV	309	205	0.01%	0.001%
74	10.087	2795	2798	2803	rBV2	572	573	0.02%	0.003%
75	10.222	2828	2840	2859	rBV	534987	825336	33.96%	4.951%
76	10.463	2910	2915	2917	rBV2	408	399	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020148.D
 Acq On : 22 Jan 2021 20:10
 Operator : SY/MD
 Sample : M1181-15DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1E34DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

77	10.543	2936	2940	2942	rBV2	488	360	0.01%	0.002%
78	10.624	2963	2965	2968	rVB	565	314	0.01%	0.002%
79	10.752	3003	3005	3013	rVB3	731	528	0.02%	0.003%
80	10.891	3045	3048	3049	rBV2	459	221	0.01%	0.001%
81	10.926	3054	3059	3065	rBV3	766	730	0.03%	0.004%
82	11.010	3083	3085	3089	rBV2	335	203	0.01%	0.001%
83	11.254	3150	3161	3182	rBV	863355	1346864	55.43%	8.079%
84	11.556	3249	3255	3257	rBV5	2542	2527	0.10%	0.015%
85	11.630	3268	3278	3300	rVB	819050	1279722	52.66%	7.676%
86	11.920	3362	3368	3374	rBV7	2669	4176	0.17%	0.025%
87	12.174	3439	3447	3450	rBV4	1209	1611	0.07%	0.010%
88	12.251	3467	3471	3474	rBV5	589	599	0.02%	0.004%
89	12.344	3499	3500	3502	rBV	499	220	0.01%	0.001%
90	12.424	3518	3525	3532	rBV7	3958	5195	0.21%	0.031%
91	12.598	3574	3579	3584	rBV4	1077	1384	0.06%	0.008%
92	12.707	3611	3613	3616	rVB3	852	382	0.02%	0.002%
93	12.740	3618	3623	3630	rVB7	2331	2777	0.11%	0.017%
94	12.785	3635	3637	3638	rBV	598	238	0.01%	0.001%
95	12.852	3653	3658	3659	rBV3	1897	1284	0.05%	0.008%
96	13.174	3755	3758	3766	rVB6	1854	1675	0.07%	0.010%
97	13.280	3783	3791	3798	rBV9	6038	9700	0.40%	0.058%
98	13.469	3848	3850	3856	rBV4	629	621	0.03%	0.004%
99	13.920	3985	3990	3998	rVB7	3396	4417	0.18%	0.026%
100	15.379	4442	4444	4445	rBV2	939	366	0.02%	0.002%




Sum of corrected areas: 16671573

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020148.D
Acq On : 22 Jan 2021 20:10
Operator : SY/MD
Sample : M1181-15DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

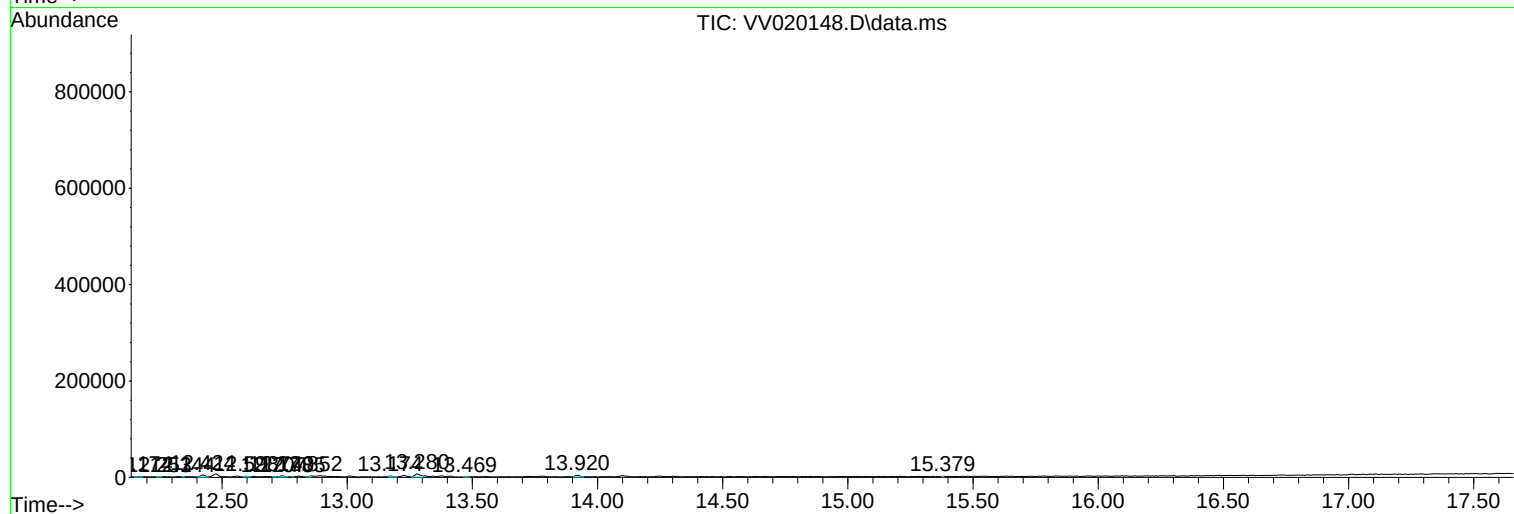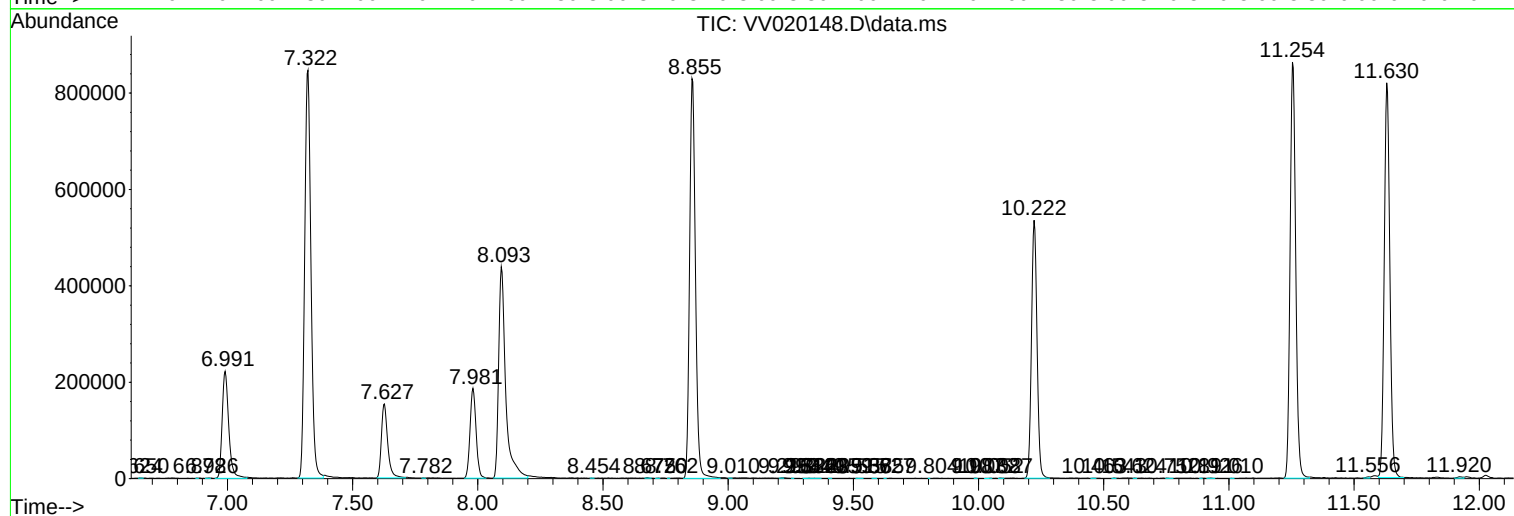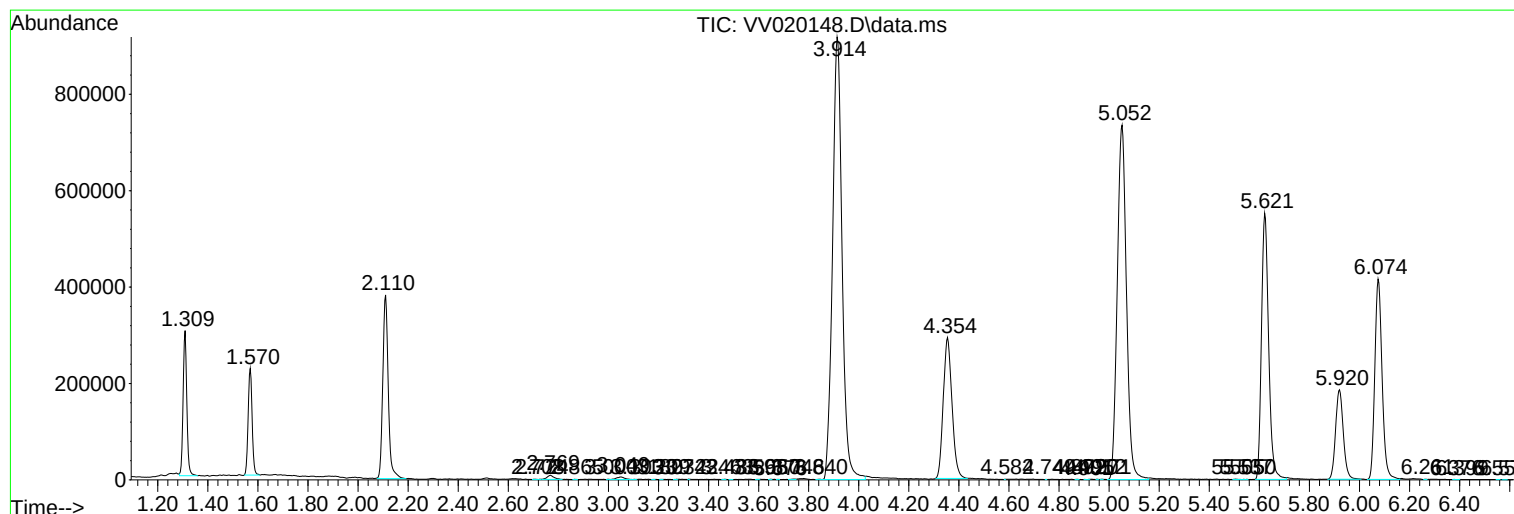

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020148.D
Acq On : 22 Jan 2021 20:10
Operator : SY/MD
Sample : M1181-15DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
Data File : VV020148.D
Acq On : 22 Jan 2021 20:10
Operator : SY/MD
Sample : M1181-15DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1E34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------