


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012221\
 Data File : VV020131.D
 Acq On : 22 Jan 2021 09:02
 Operator : SY/MD
 Sample : BFB86
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB86

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis
 Last Update : Sat Jan 23 00:14:09 2021

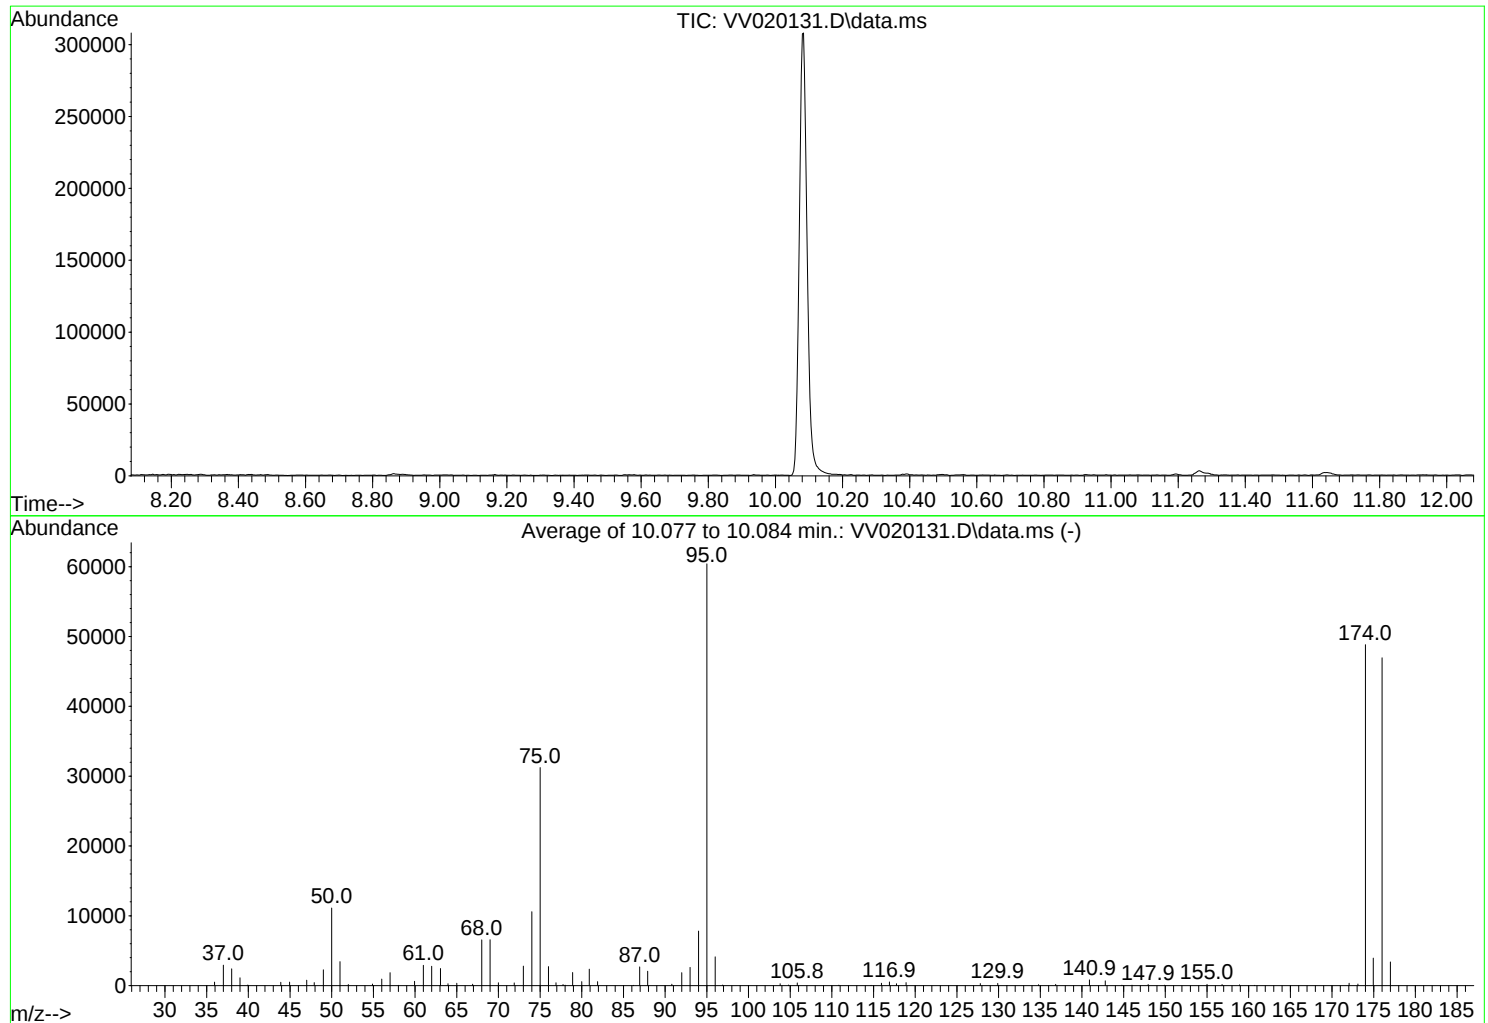

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	11110	PASS
75	95	30	80	51.7	31245	PASS
95	95	100	100	100.0	60408	PASS
96	95	5	9	6.8	4114	PASS
173	174	0.00	2	0.5	225	PASS
174	95	50	120	80.9	48840	PASS
175	174	5	9	8.1	3948	PASS
176	174	95	101	96.1	46957	PASS
177	176	5	9	7.2	3399	PASS

m/z	Abundance
40.00	139.0
43.90	248.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
35.90	528.0
37.00	2612.0
38.00	2344.0
39.00	1019.0
40.00	184.0
44.00	660.0
45.00	559.0
47.00	853.0
47.90	432.0
49.00	2221.0
50.00	10814.0
51.00	3446.0
52.00	183.0
54.90	205.0
56.00	896.0
57.00	1699.0
58.00	119.0
59.90	689.0
61.00	2746.0
62.00	2454.0
63.10	2433.0
63.90	290.0
65.00	282.0
66.80	165.0
68.00	6527.0
69.00	6438.0
70.00	386.0
71.90	340.0
73.00	2663.0
74.00	9775.0
75.00	29928.0
76.00	2753.0
76.90	484.0
78.00	189.0
78.90	1686.0
80.00	550.0
80.90	2285.0
81.90	569.0
86.90	2878.0
87.90	1980.0
90.80	181.0
92.00	1774.0
93.00	2396.0
94.00	7443.0
95.00	56448.0
96.00	3709.0
96.90	161.0
103.80	281.0
104.80	141.0
105.80	366.0
116.00	327.0
116.90	480.0
117.80	254.0
118.90	389.0
127.70	308.0
129.90	266.0
134.80	161.0
137.00	147.0
140.90	837.0
142.80	618.0
146.00	103.0
148.00	147.0
149.90	119.0
155.00	197.0
156.80	117.0
158.90	119.0
160.70	108.0
172.20	320.0
174.00	44280.0
175.00	3819.0
176.00	42312.0
177.00	3103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	525.0
37.00	3046.0
38.00	2431.0
39.00	1145.0
39.90	240.0
44.00	763.0
45.00	478.0
47.00	821.0
47.90	452.0
49.00	2283.0
50.00	11446.0
51.00	3549.0
52.00	156.0
54.90	230.0
56.00	986.0
57.00	1975.0
59.90	633.0
61.00	2982.0
62.00	2788.0
63.00	2578.0
63.90	280.0
65.00	362.0
66.90	224.0
68.00	6699.0
69.00	6829.0
70.00	413.0
71.90	408.0
73.00	2933.0
74.00	10913.0
75.00	32216.0
76.00	2800.0
76.90	419.0
77.70	217.0
78.90	1892.0
80.00	584.0
80.90	2444.0
81.90	577.0
86.90	2807.0
87.90	2069.0
90.80	210.0
92.00	1949.0
93.00	2658.0
94.00	8072.0
95.00	62632.0
96.00	4250.0
96.90	114.0
103.80	274.0
104.80	123.0
105.90	417.0
110.80	105.0
115.90	364.0
116.90	578.0
117.70	306.0
118.90	453.0
127.80	297.0
129.90	355.0
134.80	132.0
136.80	186.0
140.90	862.0
142.80	692.0
144.80	113.0
146.00	122.0
148.00	178.0
149.90	105.0
155.00	207.0
156.80	173.0
158.90	136.0
172.00	332.0
174.00	50456.0
175.00	4091.0
176.00	48464.0
177.00	3555.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	483.0
37.00	3114.0
38.00	2434.0
39.00	1182.0
39.90	250.0
43.90	763.0
44.90	478.0
47.00	684.0
47.90	411.0
49.00	2305.0
50.00	11070.0
51.00	3349.0
52.00	112.0
54.90	253.0
56.00	965.0
57.00	1915.0
60.00	516.0
61.00	3018.0
62.00	3056.0
63.00	2357.0
64.00	227.0
65.00	416.0
67.00	261.0
68.00	6432.0
69.00	6469.0
70.00	466.0
71.90	431.0
73.00	2801.0
74.00	11096.0
75.00	31592.0
76.00	2647.0
76.90	347.0
77.80	241.0
78.90	2070.0
80.00	594.0
80.90	2323.0
81.90	569.0
86.20	134.0
87.00	2388.0
87.90	2157.0
90.80	252.0
92.00	1831.0
93.00	2772.0
94.00	7927.0
95.00	62144.0
96.00	4383.0
103.80	262.0
105.90	392.0
110.90	132.0
114.70	114.0
115.90	370.0
116.90	559.0
117.80	274.0
118.90	445.0
127.90	298.0
129.90	369.0
131.00	101.0
134.80	119.0
136.80	216.0
140.90	799.0
142.80	746.0
144.80	123.0
147.80	157.0
155.00	171.0
156.80	200.0
158.90	111.0
172.00	413.0
173.10	675.0
174.00	51784.0
174.90	3933.0
176.00	50096.0
177.00	3540.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86