

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012224\
 Data File : VW033801.D
 Acq On : 22 Jan 2024 14:36
 Operator : SY/MD
 Sample : P1189-25
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMM1

Quant Time: Jan 22 23:44:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 22 23:41:48 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	226092	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	208291	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	104784	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	72077	41.480	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	82.960%	
7) Chloroethane-d5	1.532	69	59424	43.184	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	86.360%	
11) 1,1-Dichloroethene-d2	2.060	65	33267	44.485	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	88.980%	
21) 2-Butanone-d5	3.783	46	80655	67.672	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	67.670%	
24) Chloroform-d	4.249	84	130987	42.158	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	84.320%	
26) 1,2-Dichloroethane-d4	4.940	65	90682	45.170	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.340%	
32) Benzene-d6	4.960	84	261995	44.244	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.480%	
36) 1,2-Dichloropropane-d6	5.989	67	81130	41.623	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	83.240%	
41) Toluene-d8	7.243	98	241767	45.314	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	90.620%	
43) trans-1,3-Dichloroprop...	7.555	79	37598	39.029	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	78.060%	
47) 2-Hexanone-d5	8.021	63	59733	73.879	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	73.880%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84	101710	40.874	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	81.740%	
66) 1,2-Dichlorobenzene-d4	11.561	152	93747	47.155	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	94.320%	
Target Compounds						
20) cis-1,2-Dichloroethene	3.822	96	3358	1.991	ug/L	97
46) Tetrachloroethene	7.915	164	664	0.552	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012224\
Data File : VV033801.D
Acq On : 22 Jan 2024 14:36
Operator : SY/MD
Sample : P1189-25
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMM1

Quant Time: Jan 22 23:44:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 22 23:41:48 2024
Response via : Initial Calibration




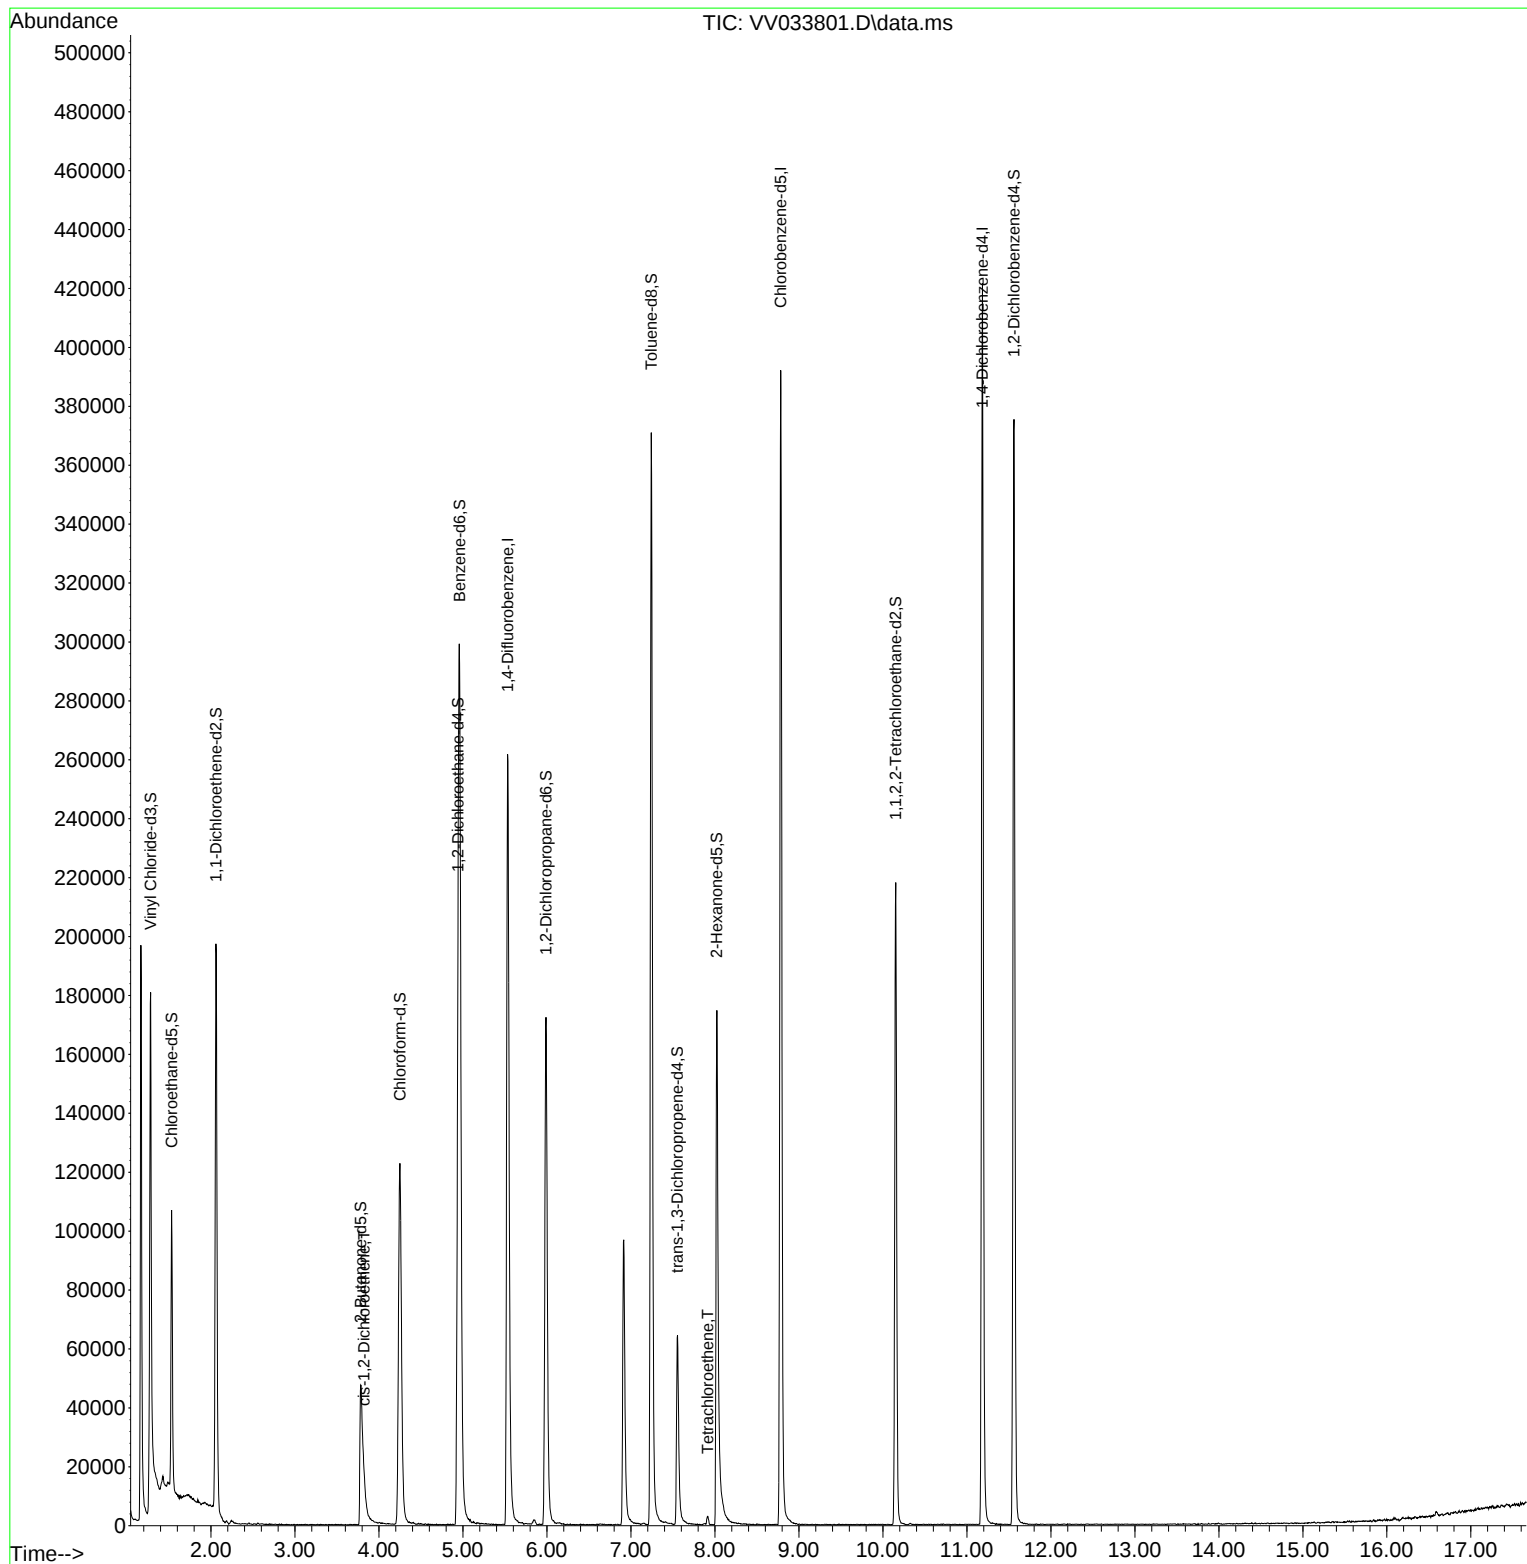


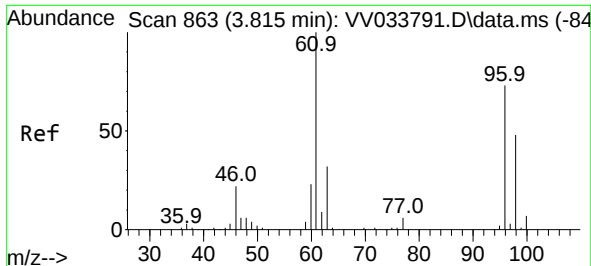

#20
cis-1,2-Dichloroethene
Concen: 1.991 ug/L
RT: 3.822 min Scan# 865
Delta R.T. 0.006 min
Lab File: VV033801.D
Acq: 22 Jan 2024 14:36

Instrument :
MSVOA_V
ClientSampleId :
DCMM1

Tgt Ion: 96 Resp: 3358
Ion Ratio Lower Upper
96 100
61 145.0 100.6 186.8
98 68.7 44.6 82.8

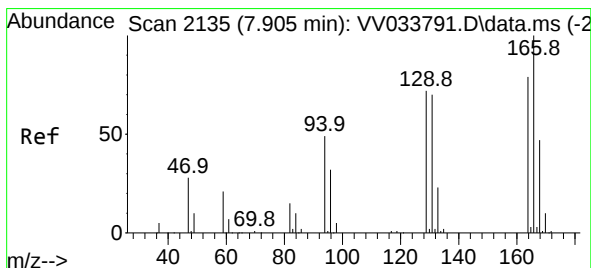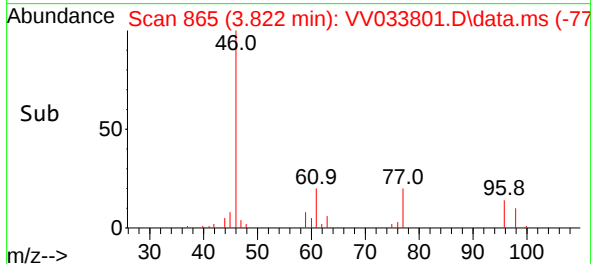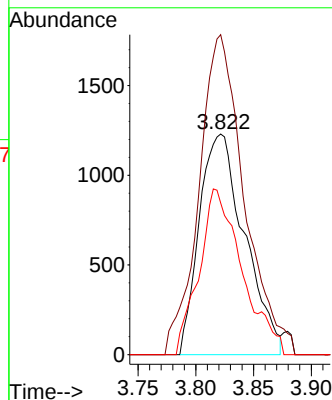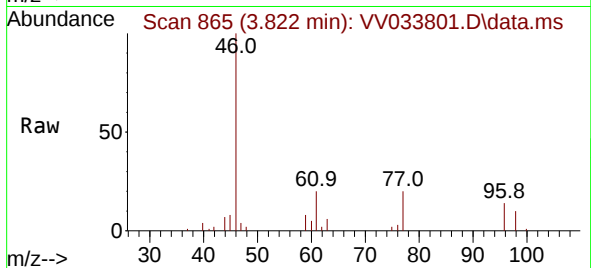

#46
Tetrachloroethene
Concen: 0.552 ug/L
RT: 7.915 min Scan# 2138
Delta R.T. 0.009 min
Lab File: VV033801.D
Acq: 22 Jan 2024 14:36

Tgt Ion: 164 Resp: 664
Ion Ratio Lower Upper
164 100
129 79.2 66.1 122.7
131 92.5 65.9 122.5
166 119.0 88.5 164.3

