

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012224\
 Data File : VV033796.D
 Acq On : 22 Jan 2024 12:37
 Operator : SY/MD
 Sample : P1189-04DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMM8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M

Title : VOC Analysis

Signal : TIC: VV033796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	33	40	51	rVB	70419	77127	9.17%	0.921%
2	1.281	63	75	109	rBV3	391152	741375	88.14%	8.857%
3	1.532	147	153	167	rVB	102973	133616	15.89%	1.596%
4	2.060	309	317	331	rVB	207672	309619	36.81%	3.699%
5	2.156	343	347	361	rVB3	6379	9405	1.12%	0.112%
6	2.243	364	374	388	rVB2	6933	12525	1.49%	0.150%
7	2.336	396	403	415	rBV2	2837	5069	0.60%	0.061%
8	2.449	427	438	459	rVB	59500	100785	11.98%	1.204%
9	2.561	464	473	486	rBV2	1990	3901	0.46%	0.047%
10	2.645	495	499	500	rBV2	227	156	0.02%	0.002%
11	2.703	507	517	532	rVB2	5988	10507	1.25%	0.126%
12	2.818	546	553	556	rBV3	291	389	0.05%	0.005%
13	3.249	684	687	692	rVV2	144	171	0.02%	0.002%
14	3.812	844	862	896	rBV2	227756	687444	81.73%	8.213%
15	4.124	956	959	962	rVB3	359	245	0.03%	0.003%
16	4.159	966	970	972	rBV3	339	287	0.03%	0.003%
17	4.256	983	1000	1036	rBV4	166527	574549	68.31%	6.864%
18	4.432	1052	1055	1060	rVB4	455	366	0.04%	0.004%
19	4.590	1096	1104	1106	rBV2	229	277	0.03%	0.003%
20	4.657	1120	1125	1127	rBV2	232	184	0.02%	0.002%
21	4.889	1192	1197	1201	rBV2	221	280	0.03%	0.003%
22	4.957	1201	1218	1243	rBV2	317830	841110	100.00%	10.049%
23	5.185	1286	1289	1292	rBV2	416	283	0.03%	0.003%
24	5.349	1338	1340	1347	rVB2	358	282	0.03%	0.003%
25	5.391	1350	1353	1359	rVB3	270	276	0.03%	0.003%
26	5.532	1386	1397	1434	rBV	263458	543739	64.65%	6.496%
27	5.754	1464	1466	1473	rVB2	181	169	0.02%	0.002%
28	5.838	1486	1492	1493	rBV3	1039	944	0.11%	0.011%
29	5.895	1504	1510	1513	rBV2	334	350	0.04%	0.004%
30	5.911	1513	1515	1521	rVB2	391	270	0.03%	0.003%
31	5.989	1521	1539	1565	rBV	186345	387078	46.02%	4.625%
32	6.227	1609	1613	1616	rVB4	405	293	0.03%	0.004%
33	6.352	1649	1652	1655	rVB3	254	159	0.02%	0.002%
34	6.374	1655	1659	1663	rBV2	231	220	0.03%	0.003%
35	6.423	1671	1674	1675	rBV2	330	221	0.03%	0.003%
36	6.583	1721	1724	1728	rBV2	363	349	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012224\
 Data File : VV033796.D
 Acq On : 22 Jan 2024 12:37
 Operator : SY/MD
 Sample : P1189-04DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMM8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.915	1816	1827	1856	rVV	103238	195714	23.27%	2.338%
38	7.037	1856	1865	1880	rVB4	4165	8818	1.05%	0.105%
39	7.120	1889	1891	1894	rBV2	264	211	0.03%	0.003%
40	7.178	1901	1909	1918	rBV	7673	12992	1.54%	0.155%
41	7.243	1918	1929	1954	rVV	389048	689663	81.99%	8.240%
42	7.365	1960	1967	1987	rVB2	12625	25063	2.98%	0.299%
43	7.554	2016	2026	2050	rBV	69066	124634	14.82%	1.489%
44	7.783	2094	2097	2103	rBV2	217	159	0.02%	0.002%
45	7.870	2117	2124	2125	rBV	580	449	0.05%	0.005%
46	8.024	2163	2172	2207	rBV	203160	393494	46.78%	4.701%
47	8.349	2271	2273	2278	rVB2	499	276	0.03%	0.003%
48	8.445	2298	2303	2306	rBV	279	284	0.03%	0.003%
49	8.783	2397	2408	2438	rBV	407165	670991	79.77%	8.017%
50	9.005	2475	2477	2483	rVB3	360	283	0.03%	0.003%
51	9.236	2546	2549	2555	rVB2	166	163	0.02%	0.002%
52	9.384	2593	2595	2604	rVB2	239	179	0.02%	0.002%
53	9.667	2676	2683	2691	rBV4	2181	4081	0.49%	0.049%
54	9.767	2711	2714	2718	rVB2	327	186	0.02%	0.002%
55	9.824	2725	2732	2734	rBV4	1350	1746	0.21%	0.021%
56	9.876	2745	2748	2750	rBV2	322	179	0.02%	0.002%
57	10.014	2783	2791	2796	rVB4	1118	1458	0.17%	0.017%
58	10.152	2816	2834	2855	rBV	239944	383525	45.60%	4.582%
59	10.287	2872	2876	2879	rVB2	257	171	0.02%	0.002%
60	10.323	2884	2887	2888	rBV	300	160	0.02%	0.002%
61	10.455	2925	2928	2929	rBV	348	184	0.02%	0.002%
62	10.548	2953	2957	2962	rVB2	211	226	0.03%	0.003%
63	10.660	2988	2992	2994	rBV2	223	198	0.02%	0.002%
64	10.731	3006	3014	3021	rBV4	946	1290	0.15%	0.015%
65	10.892	3057	3064	3070	rBV4	1591	2436	0.29%	0.029%
66	10.947	3079	3081	3087	rVB	214	238	0.03%	0.003%
67	10.998	3089	3097	3098	rBV4	1055	950	0.11%	0.011%
68	11.130	3134	3138	3141	rBV3	520	383	0.05%	0.005%
69	11.185	3144	3155	3178	rBV	446201	692754	82.36%	8.277%
70	11.291	3179	3188	3196	rVB4	13293	19836	2.36%	0.237%
71	11.561	3250	3272	3299	rBV	416201	660010	78.47%	7.885%
72	11.699	3312	3315	3317	rBV2	274	157	0.02%	0.002%
73	11.725	3317	3323	3335	rVB4	1949	3194	0.38%	0.038%
74	11.824	3351	3354	3356	rBV	239	150	0.02%	0.002%
75	11.844	3358	3360	3367	rVB2	298	230	0.03%	0.003%
76	11.937	3384	3389	3391	rBV	324	201	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012224\
 Data File : VV033796.D
 Acq On : 22 Jan 2024 12:37
 Operator : SY/MD
 Sample : P1189-04DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMM8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.194	3462	3469	3471	rBV3	1415	1421	0.17%	0.017%
78	12.828	3659	3666	3672	rVV5	1287	1756	0.21%	0.021%
79	12.873	3672	3680	3694	rVB	5726	9530	1.13%	0.114%
80	12.992	3714	3717	3720	rBV	302	226	0.03%	0.003%
81	13.104	3742	3752	3758	rVB5	1723	2440	0.29%	0.029%
82	13.210	3783	3785	3788	rVB	343	182	0.02%	0.002%
83	13.281	3805	3807	3813	rVV3	275	226	0.03%	0.003%
84	13.342	3823	3826	3830	rVB2	241	167	0.02%	0.002%
85	13.451	3853	3860	3861	rVV2	578	565	0.07%	0.007%
86	13.461	3861	3863	3867	rVB3	819	486	0.06%	0.006%
87	13.773	3957	3960	3961	rBV	463	311	0.04%	0.004%
88	13.898	3997	3999	4003	rVB2	277	194	0.02%	0.002%
89	13.927	4004	4008	4011	rBV2	508	420	0.05%	0.005%
90	13.966	4018	4020	4023	rBV2	295	245	0.03%	0.003%
91	14.046	4042	4045	4048	rVB3	204	151	0.02%	0.002%
92	14.069	4049	4052	4056	rVB2	255	160	0.02%	0.002%
93	14.091	4056	4059	4063	rBV	266	243	0.03%	0.003%
94	14.117	4063	4067	4069	rBV3	203	156	0.02%	0.002%
95	14.178	4083	4086	4089	rBV2	263	207	0.02%	0.002%
96	14.268	4110	4114	4116	rBV3	365	279	0.03%	0.003%
97	14.352	4131	4140	4151	rVB6	4265	7017	0.83%	0.084%
98	14.673	4237	4240	4242	rBV2	256	164	0.02%	0.002%
99	14.792	4270	4277	4283	rBV3	1024	1600	0.19%	0.019%
100	16.345	4758	4760	4763	rBV3	820	562	0.07%	0.007%




Sum of corrected areas: 8370044

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012224\
Data File : VV033796.D
Acq On : 22 Jan 2024 12:37
Operator : SY/MD
Sample : P1189-04DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMM8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

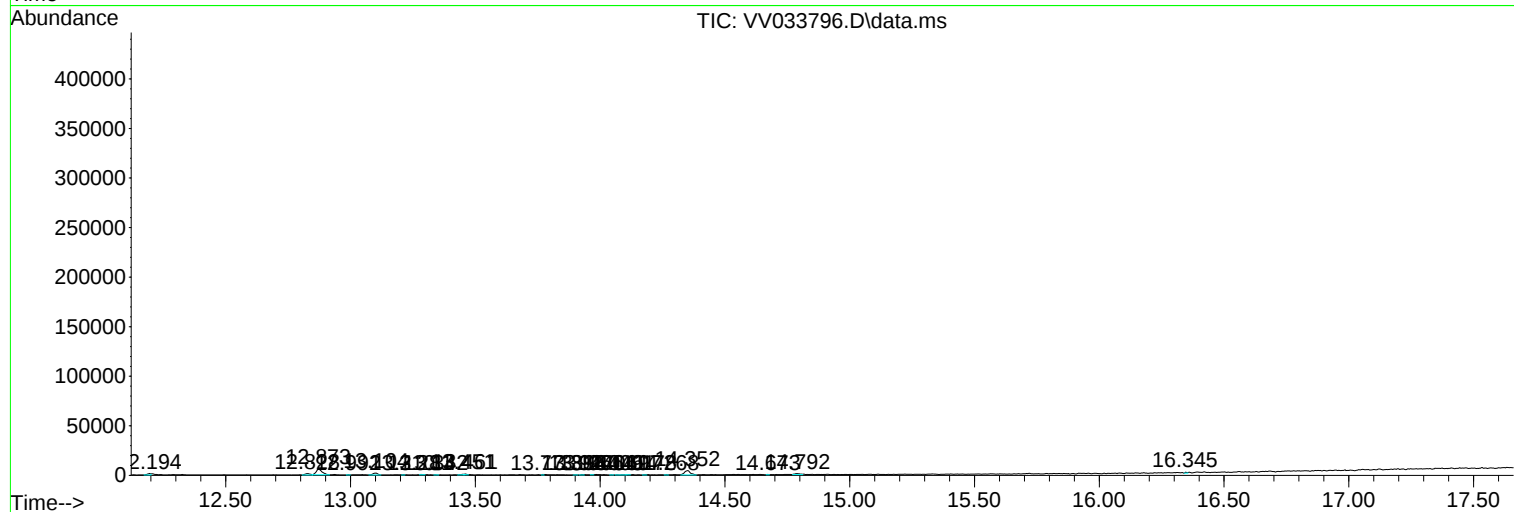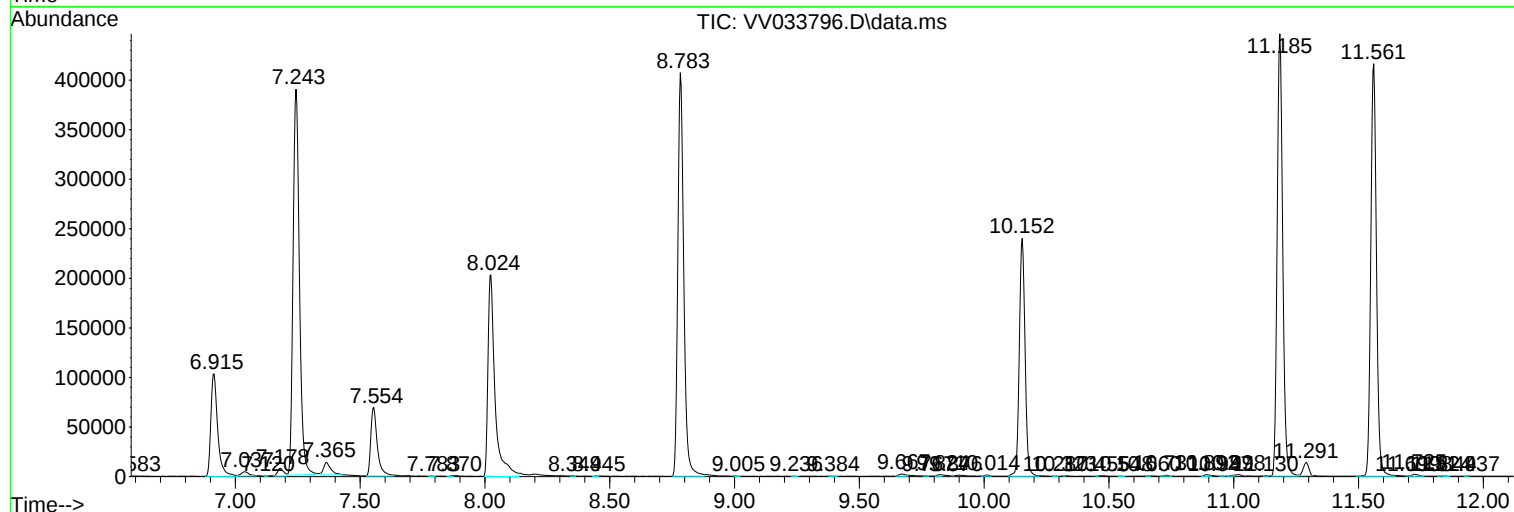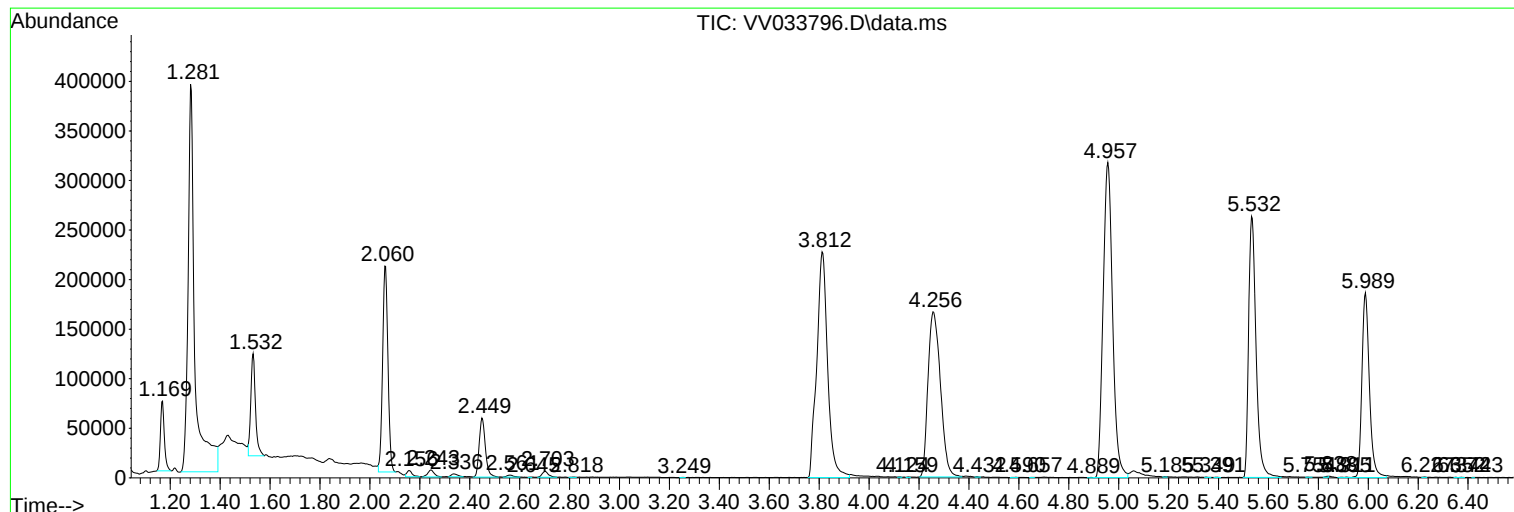

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012224\
Data File : VV033796.D
Acq On : 22 Jan 2024 12:37
Operator : SY/MD
Sample : P1189-04DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMM8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012224\
Data File : VV033796.D
Acq On : 22 Jan 2024 12:37
Operator : SY/MD
Sample : P1189-04DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMM8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
