


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012224\
Data File : VV033790.D
Acq On : 22 Jan 2024 09:13
Operator : SY/MD
Sample : BFB255
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB255

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Title : VOC Analysis
Last Update : Wed Jan 24 02:00:55 2024

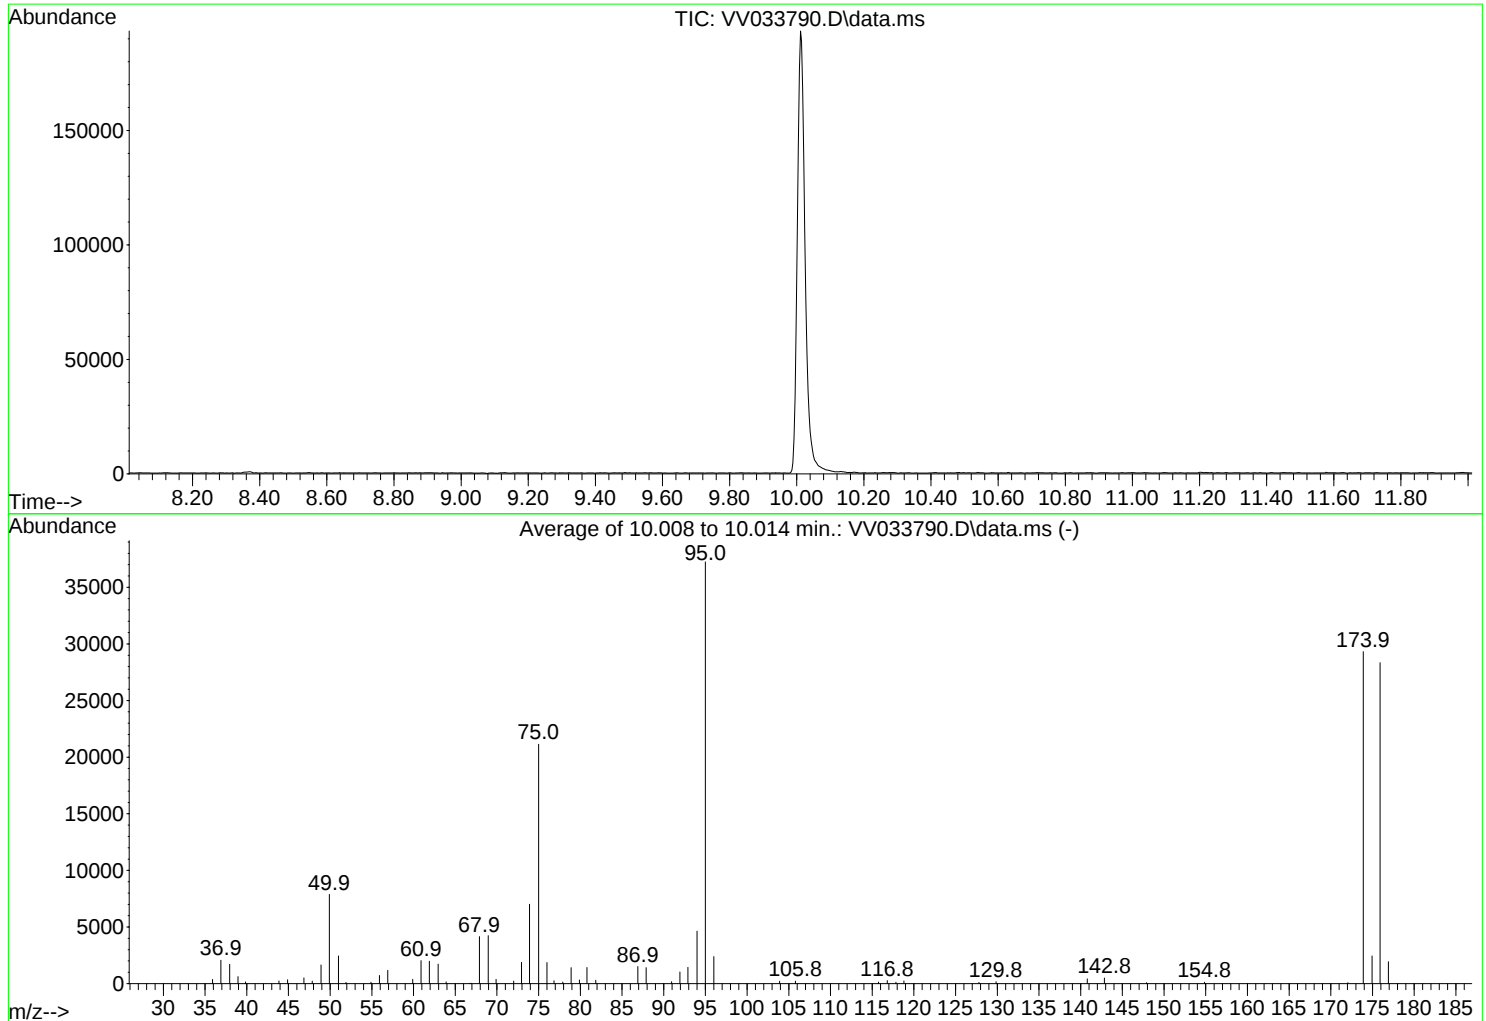

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	7884	PASS
75	95	30	80	56.7	21133	PASS
95	95	100	100	100.0	37248	PASS
96	95	5	9	6.4	2393	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.7	29325	PASS
175	174	5	9	8.4	2449	PASS
176	174	95	105	96.7	28347	PASS
177	176	5	10	6.8	1930	PASS

m/z	Abundance
39.80	186.0
43.80	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
35.90	352.0
36.90	2092.0
38.00	1590.0
38.90	630.0
39.90	336.0
43.90	380.0
44.90	316.0
46.80	429.0
47.80	245.0
48.90	1628.0
49.90	7658.0
51.00	2341.0
51.90	126.0
54.90	134.0
55.90	666.0
56.90	1146.0
59.90	385.0
60.90	2011.0
61.90	1902.0
62.90	1651.0
63.80	180.0
67.90	4016.0
69.00	3925.0
69.90	320.0
71.90	204.0
73.00	1787.0
73.90	6694.0
75.00	20368.0
76.00	1708.0
76.80	232.0
77.90	161.0
78.90	1272.0
79.80	351.0
80.80	1344.0
81.90	292.0
86.90	1476.0
87.90	1362.0
90.90	168.0
91.90	972.0
92.90	1433.0
94.00	4411.0
95.00	35528.0
96.00	2396.0
103.90	203.0
105.80	244.0
115.90	147.0
116.80	243.0
117.90	115.0
118.80	208.0
127.80	122.0
129.90	160.0
140.80	392.0
142.80	472.0
154.80	118.0
172.00	122.0
173.90	27400.0
175.00	2362.0
175.90	26144.0
176.90	1770.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
35.90	376.0
36.90	2134.0
37.90	1766.0
39.00	645.0
39.90	356.0
43.90	415.0
44.90	344.0
46.90	515.0
47.80	218.0
48.90	1721.0
49.90	8243.0
51.00	2531.0
51.90	117.0
54.90	121.0
55.90	759.0
56.90	1214.0
59.90	391.0
60.90	2109.0
61.90	2048.0
62.90	1800.0
63.90	146.0
66.70	104.0
67.90	4293.0
68.90	4405.0
69.90	402.0
72.00	228.0
72.90	1947.0
73.90	7190.0
75.00	22040.0
76.00	1917.0
76.80	262.0
77.90	145.0
78.90	1477.0
79.90	329.0
80.80	1477.0
81.90	316.0
86.90	1570.0
87.90	1452.0
90.90	166.0
92.00	1058.0
92.90	1488.0
94.00	4815.0
95.00	38664.0
96.00	2451.0
103.90	225.0
105.80	233.0
115.70	142.0
116.80	273.0
117.80	131.0
118.80	254.0
127.80	124.0
129.80	180.0
140.80	447.0
142.90	517.0
147.90	122.0
154.80	146.0
172.10	120.0
173.90	30464.0
174.90	2536.0
175.90	29344.0
176.90	2010.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255

m/z	Abundance
35.90	378.0
36.90	1952.0
37.90	1757.0
39.00	598.0
39.90	337.0
43.90	384.0
44.90	366.0
46.90	582.0
47.90	209.0
48.90	1630.0
49.90	7751.0
51.00	2458.0
51.90	114.0
54.90	119.0
55.90	763.0
56.90	1155.0
59.90	365.0
60.90	2008.0
61.90	1987.0
63.00	1711.0
64.00	144.0
66.90	130.0
67.90	4149.0
68.90	4383.0
69.90	415.0
72.10	232.0
72.90	1918.0
73.90	7128.0
75.00	20992.0
76.00	1963.0
76.90	260.0
77.90	133.0
78.90	1482.0
80.00	297.0
80.80	1473.0
81.80	308.0
86.90	1478.0
87.90	1410.0
91.00	171.0
91.90	1071.0
92.90	1415.0
94.00	4694.0
95.00	37552.0
96.00	2332.0
103.90	221.0
105.80	206.0
115.70	137.0
116.80	271.0
117.80	144.0
118.80	271.0
127.80	107.0
129.80	168.0
140.80	438.0
142.90	492.0
147.90	147.0
154.90	136.0
173.90	30112.0
174.90	2448.0
175.90	29552.0
176.90	2009.0

Instrument :
MSVOA_V
ClientSampleId :
BFB255