




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012225\
Data File : VV038501.D
Acq On : 22 Jan 2025 15:57
Operator : SY/MD
Sample : Q1137-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAB3

Manual IntegrationsAPPROVED

Quant Time: Jan 23 01:40:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 23 01:38:03 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 01/24/2025
Supervised By :Semsettin Yesilyurt 01/24/2025

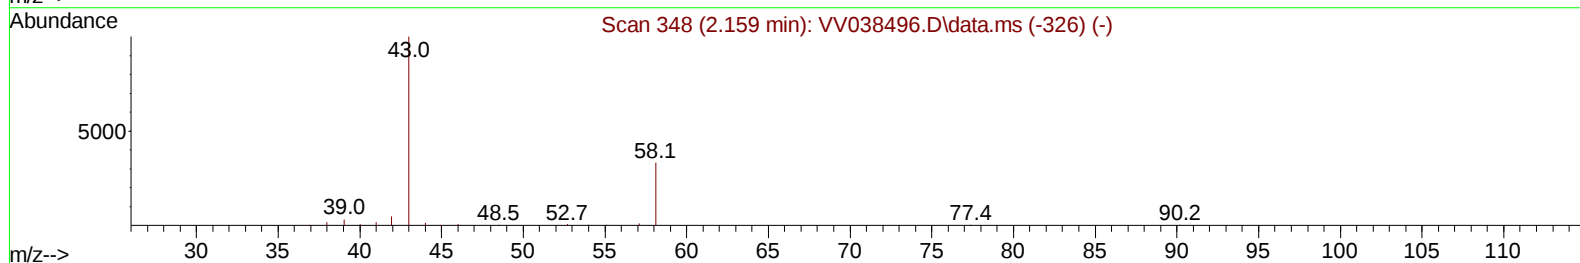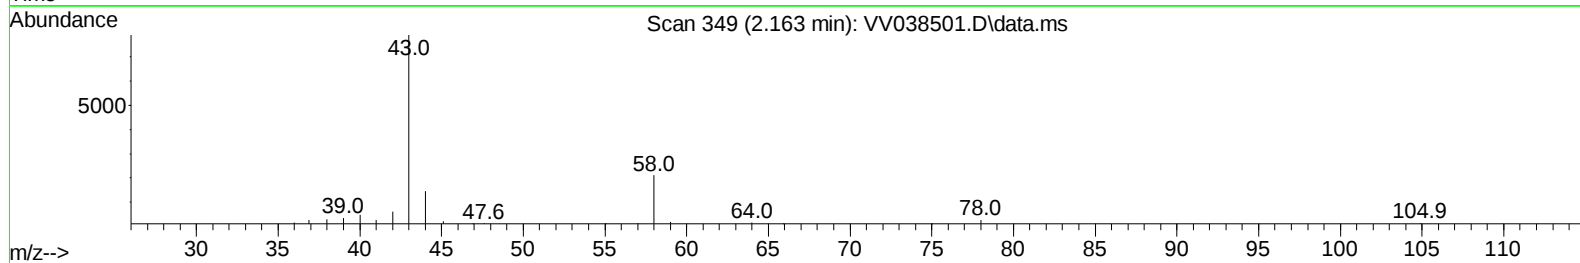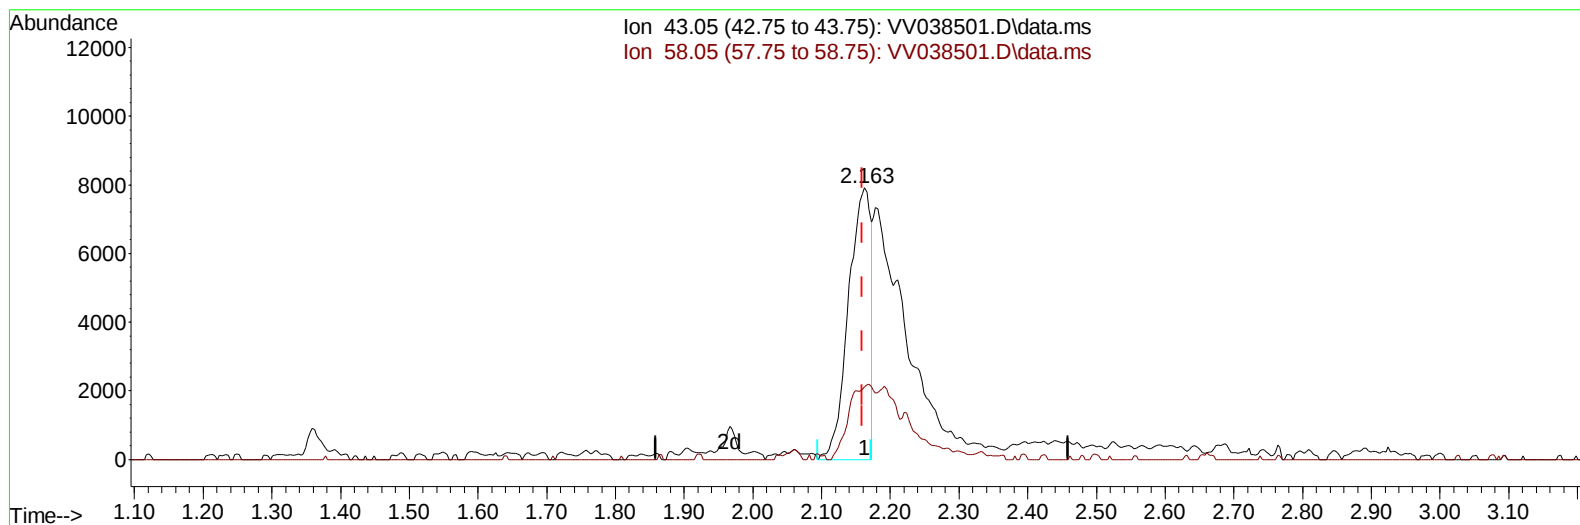

TIC: VV038501.D\data.ms

(13) Acetone (T)

2.163min (+ 0.003) 8.66 ug/L

response 17601

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.60	32.11
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012225\
Data File : VV038501.D
Acq On : 22 Jan 2025 15:57
Operator : SY/MD
Sample : Q1137-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAB3

Manual IntegrationsAPPROVED

Quant Time: Jan 23 01:40:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 23 01:38:03 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 01/24/2025
Supervised By :Semsettin Yesilyurt 01/24/2025

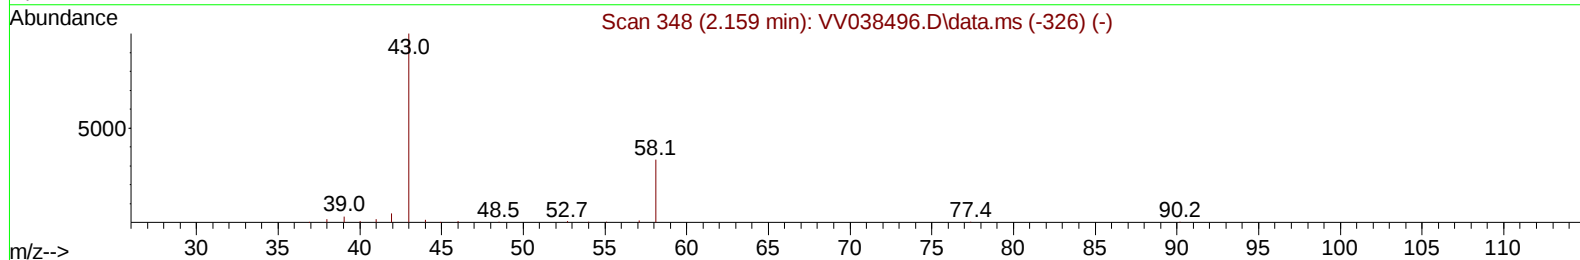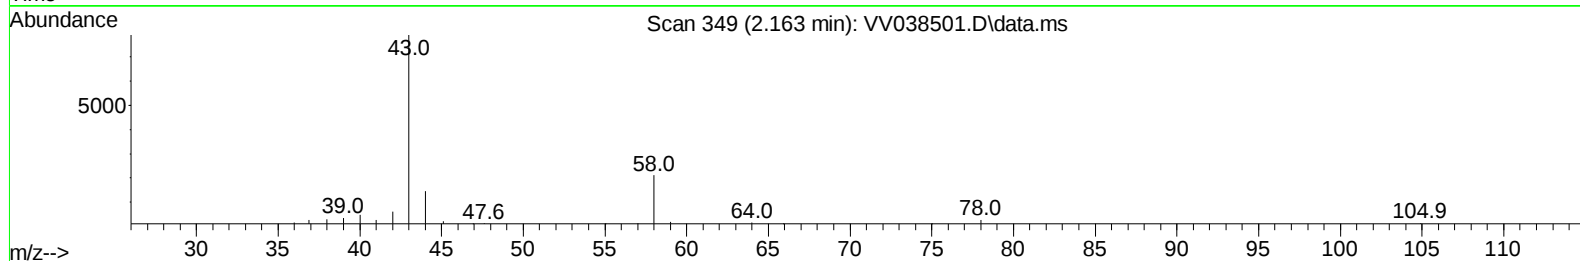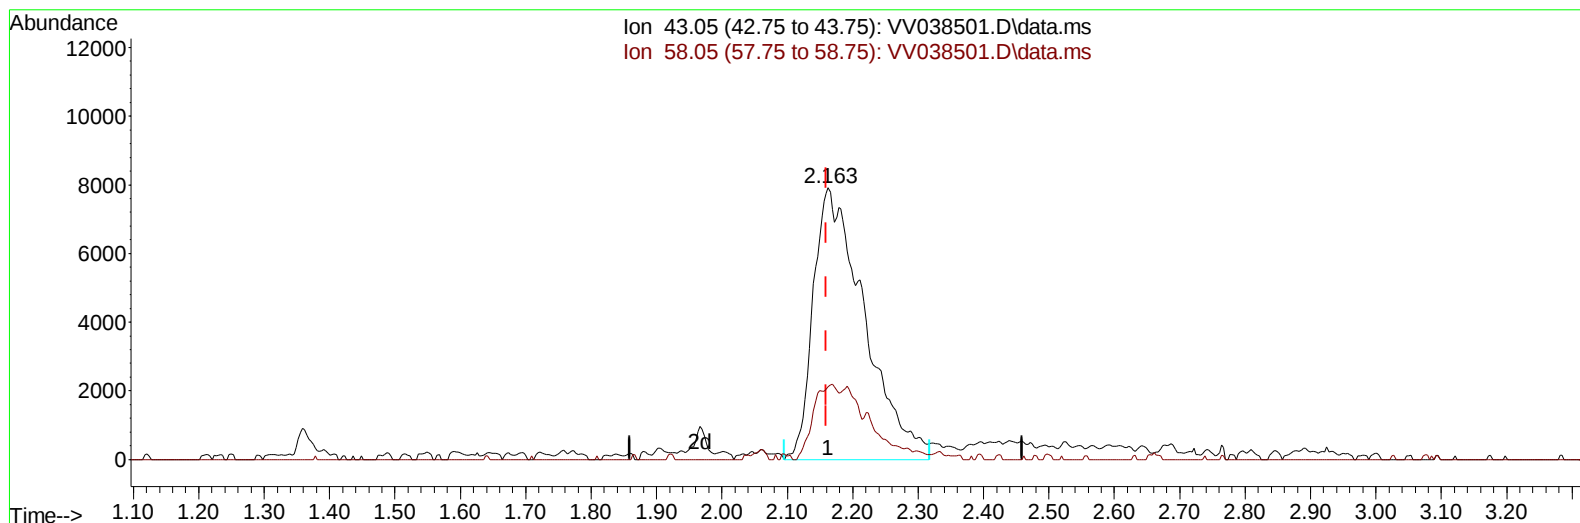

TIC: VV038501.D\data.ms

(13) Acetone (T)

2.163min (+ 0.003) 21.05 ug/L m

response 42800

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.60	13.20
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012225\
 Data File : VV038501.D
 Acq On : 22 Jan 2025 15:57
 Operator : SY/MD
 Sample : Q1137-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAB3

Manual IntegrationsAPPROVED

Quant Time: Jan 23 01:40:37 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 23 01:38:03 2025
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 01/24/2025
 Supervised By :Semsettin Yesilyurt 01/24/2025

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.532	114		150640	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117		165369	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152		67962	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		46181	3.717	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	74.400%		
7) Chloroethane-d5	1.532	69		44165	4.234	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	84.600%		
11) 1,1-Dichloroethene-d2	2.056	65		21584	3.856	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	77.200%		
20) 2-Butanone-d5	3.838	46		119679	45.805	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130		Recovery =	91.620%		
24) Chloroform-d	4.243	84		103729	4.455	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	89.200%		
26) 1,2-Dichloroethane-d4	4.941	65		51991	4.873	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	97.400%		
32) Benzene-d6	4.953	84		183546	4.030	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	80.600%		
36) 1,2-Dichloropropane-d6	5.986	67		63974	4.621	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	92.400%		
41) Toluene-d8	7.239	98		140977	3.446	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	69.000%#		
43) trans-1,3-Dichloroprop...	7.561	79		19286	3.808	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	76.200%		
46) 2-Hexanone-d5	8.027	63		72693	36.385	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	72.760%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84		54684	4.982	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	99.600%		
66) 1,2-Dichlorobenzene-d4	11.554	152		57387	4.989	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	99.800%		
Target Compounds							
3) Chloromethane	1.214	50		585074	33.887	ug/L	99
13) Acetone	2.163	43		42800m	21.053	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012225\
Data File : VV038501.D
Acq On : 22 Jan 2025 15:57
Operator : SY/MD
Sample : Q1137-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAB3

Manual IntegrationsAPPROVED

Quant Time: Jan 23 01:40:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 23 01:38:03 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 01/24/2025
Supervised By :Semsettin Yesilyurt 01/24/2025

