
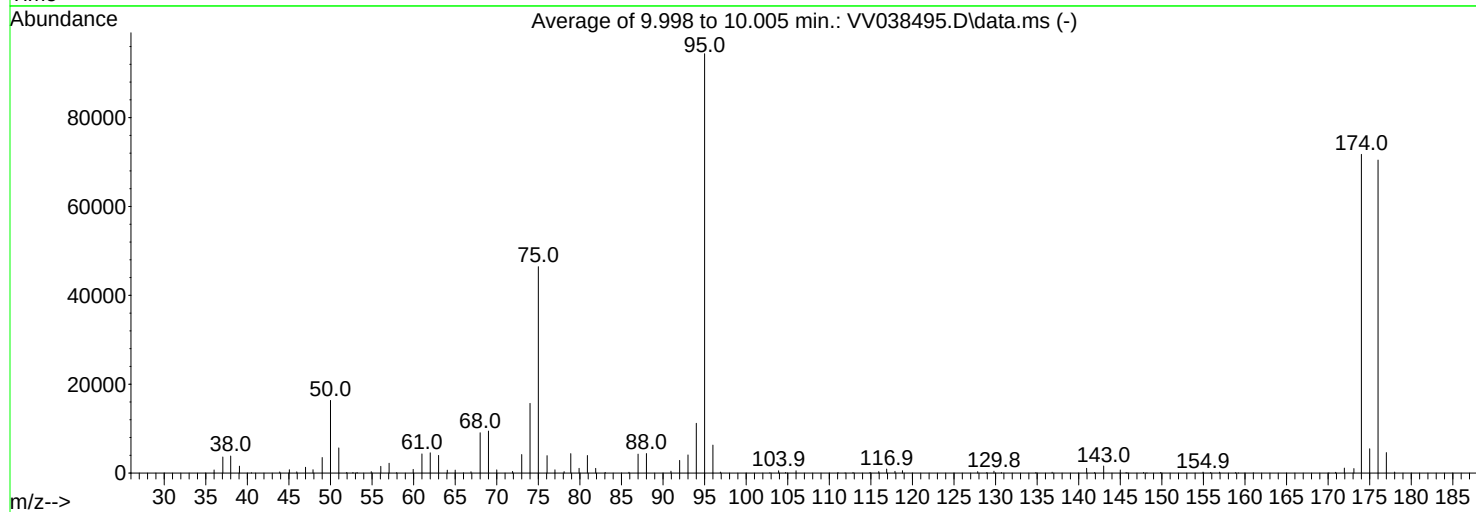


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012225\
Data File : VV038495.D
Acq On : 22 Jan 2025 12:43
Operator : SY/MD
Sample : BFB400
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB400

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jan 24 00:30:49 2025

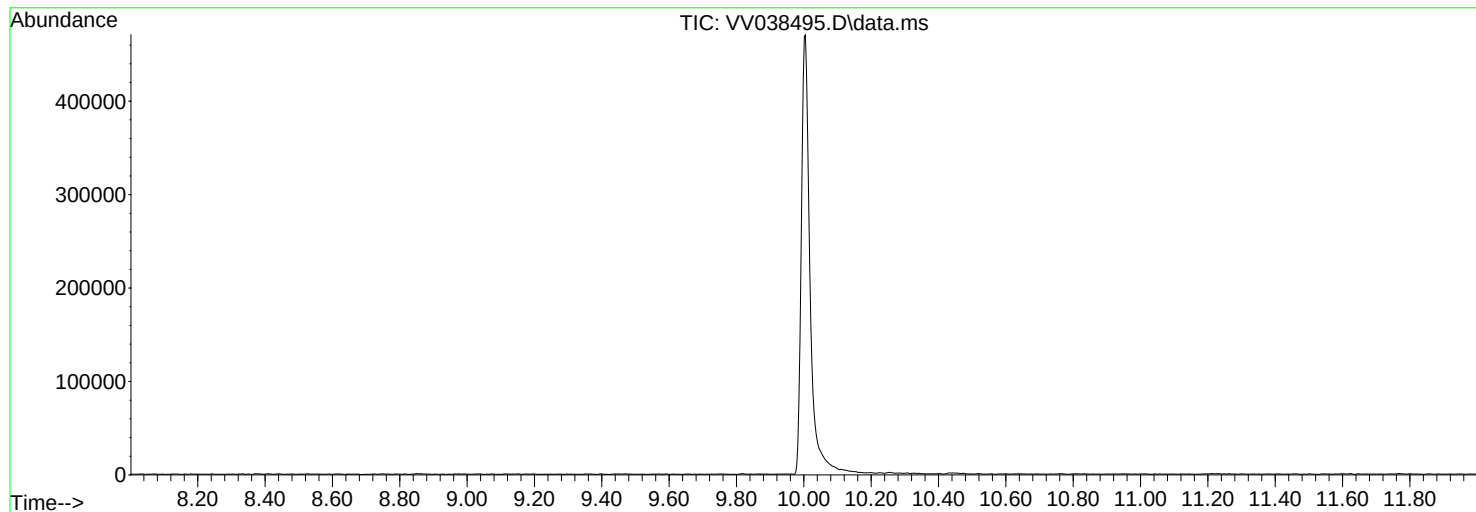

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	16363	PASS
75	95	30	80	49.2	46448	PASS
95	95	100	100	100.0	94379	PASS
96	95	5	9	6.7	6298	PASS
173	174	0.00	2	1.4	1017	PASS
174	95	50	120	76.0	71733	PASS
175	174	5	9	7.6	5470	PASS
176	174	95	105	98.2	70448	PASS
177	176	5	10	6.5	4613	PASS

m/z	Abundance
40.00	463.0
42.00	114.0
43.90	423.0

Instrument :
MSVOA_V
ClientSampleId :
BFB400

m/z	Abundance
36.00	651.0
37.10	3375.0
38.00	3774.0
39.00	1592.0
39.90	434.0
43.90	700.0
45.00	738.0
45.90	222.0
47.00	1223.0
47.90	803.0
49.00	3263.0
50.00	15546.0
51.00	5400.0
52.00	168.0
52.70	150.0
53.20	122.0
54.90	255.0
56.00	1439.0
57.10	2139.0
57.90	159.0
59.90	841.0
61.00	4041.0
62.00	4153.0
63.00	3884.0
64.00	657.0
65.00	616.0
66.00	119.0
66.90	238.0
68.00	8509.0
69.00	9052.0
70.00	677.0
71.90	383.0
73.00	4120.0
74.00	14918.0
75.00	44208.0
76.10	3716.0
77.00	776.0
78.10	509.0
78.90	4027.0
79.90	978.0
80.90	3874.0
81.90	976.0
83.00	105.0
86.00	192.0
87.00	3894.0
88.00	4102.0
90.90	399.0
92.00	2592.0
93.00	3933.0
94.00	10348.0
95.00	87888.0
96.00	5772.0
96.90	231.0
103.90	499.0
104.70	161.0
106.00	436.0
111.00	109.0
112.80	151.0
114.90	141.0
115.90	386.0
116.90	890.0
117.90	451.0
118.80	537.0
127.80	286.0
129.00	141.0
129.80	404.0
130.70	103.0
134.90	141.0
136.80	193.0
141.00	973.0
143.00	1523.0
145.00	619.0
145.70	139.0
147.80	109.0
148.20	134.0
149.80	140.0
154.90	265.0
155.90	121.0
156.90	195.0
158.90	191.0
171.90	1000.0
173.10	912.0
174.00	64416.0
175.00	4959.0
176.00	64264.0
177.00	4245.0
178.00	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB400

m/z	Abundance
36.00	724.0
37.00	3685.0
38.00	3962.0
39.00	1584.0
39.90	412.0
44.00	658.0
45.10	793.0
45.90	311.0
47.00	1379.0
47.90	790.0
49.00	3622.0
50.00	16968.0
51.00	5850.0
51.90	125.0
52.70	154.0
53.20	161.0
54.90	345.0
56.00	1518.0
57.00	2239.0
58.00	112.0
59.90	841.0
61.00	4398.0
62.00	4685.0
63.00	4019.0
64.00	680.0
65.00	702.0
66.90	326.0
68.00	9394.0
69.00	9827.0
70.00	749.0
71.90	381.0
73.00	4299.0
74.00	16087.0
75.00	48032.0
76.10	4070.0
77.00	763.0
78.10	476.0
78.90	4545.0
79.90	1121.0
80.90	4051.0
81.90	1124.0
83.10	150.0
85.90	168.0
87.00	4348.0
88.00	4651.0
90.90	417.0
92.00	2907.0
93.00	4196.0
94.00	11635.0
95.00	97712.0
96.00	6566.0
96.90	216.0
102.90	138.0
103.90	545.0
104.70	147.0
106.00	565.0
111.00	126.0
112.90	149.0
114.90	162.0
116.00	333.0
116.90	946.0
117.90	396.0
118.80	549.0
127.80	331.0
128.90	141.0
129.80	463.0
130.70	122.0
134.90	150.0
136.80	205.0
141.00	1116.0
141.90	135.0
143.00	1618.0
145.00	743.0
145.70	150.0
147.80	147.0
149.80	157.0
154.90	217.0
155.80	151.0
156.90	205.0
158.80	138.0
170.90	211.0
171.90	1199.0
173.10	1032.0
174.00	73840.0
175.00	5548.0
176.00	72896.0
177.00	4835.0
178.00	249.0

Instrument :
MSVOA_V
ClientSampleId :
BFB400

m/z	Abundance
36.00	728.0
37.00	3797.0
38.00	3778.0
39.10	1496.0
39.90	401.0
40.50	237.0
44.00	681.0
45.10	726.0
46.00	326.0
47.00	1339.0
47.90	663.0
49.00	3629.0
50.00	16576.0
51.00	5730.0
51.90	152.0
52.70	112.0
53.20	128.0
54.90	385.0
56.10	1598.0
57.00	2261.0
60.00	816.0
61.00	4490.0
62.00	4858.0
63.00	4029.0
64.10	651.0
65.00	705.0
66.90	369.0
68.00	9321.0
69.00	9497.0
70.00	759.0
71.90	337.0
73.00	4100.0
74.00	16063.0
75.00	47104.0
76.00	3981.0
77.00	676.0
78.90	4543.0
79.90	1109.0
80.90	3944.0
81.90	1082.0
83.10	156.0
85.80	180.0
87.00	4560.0
88.00	4455.0
91.00	477.0
92.00	3074.0
93.00	4117.0
94.00	11648.0
95.00	97536.0
96.00	6557.0
96.90	233.0
102.80	131.0
103.90	537.0
104.80	122.0
106.00	552.0
111.10	114.0
111.90	102.0
112.90	118.0
114.90	146.0
116.00	309.0
116.90	880.0
117.90	342.0
118.80	542.0
127.90	352.0
128.90	146.0
129.80	434.0
130.70	136.0
134.80	150.0
136.80	193.0
140.90	1120.0
141.90	183.0
143.00	1631.0
145.00	745.0
145.70	135.0
145.90	134.0
147.80	183.0
149.90	125.0
155.00	187.0
155.80	113.0
157.00	213.0
159.20	122.0
161.00	121.0
170.10	101.0
170.90	316.0
172.00	1195.0
173.10	1108.0
174.00	76944.0
175.00	5902.0
176.00	74184.0
177.00	4759.0
178.00	266.0

Instrument :
MSVOA_V
ClientSampleId :
BFB400