

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012323\
 Data File : VW029905.D
 Acq On : 23 Jan 2023 16:05
 Operator : SY/MD
 Sample : 01216-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jan 24 01:34:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 24 01:33:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	169631	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	170669	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	91213	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	64337	5.000	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.000%
7) Chloroethane-d5	1.565	69	60731	5.694	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.800%
11) 1,1-Dichloroethene-d2	2.105	63	85227	3.634	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.600%
20) 2-Butanone-d5	3.899	46	124062	54.402	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.800%
24) Chloroform-d	4.339	84	120289	5.097	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%
26) 1,2-Dichloroethane-d4	5.024	65	52635	5.266	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.400%
32) Benzene-d6	5.044	84	235299	4.648	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%
36) 1,2-Dichloropropane-d6	6.063	67	78864	5.323	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.400%
41) Toluene-d8	7.307	98	190283	4.060	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.200%
43) trans-1,3-Dichloroprop...	7.616	79	21724	4.015	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.200%
46) 2-Hexanone-d5	8.085	63	102047	46.322	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.640%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	56805	5.232	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.600%
66) 1,2-Dichlorobenzene-d4	11.612	152	76281	4.600	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.000%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	7654	0.425	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029905.D
Acq On : 23 Jan 2023 16:05
Operator : SY/MD
Sample : 01216-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Jan 24 01:34:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 24 01:33:02 2023
Response via : Initial Calibration

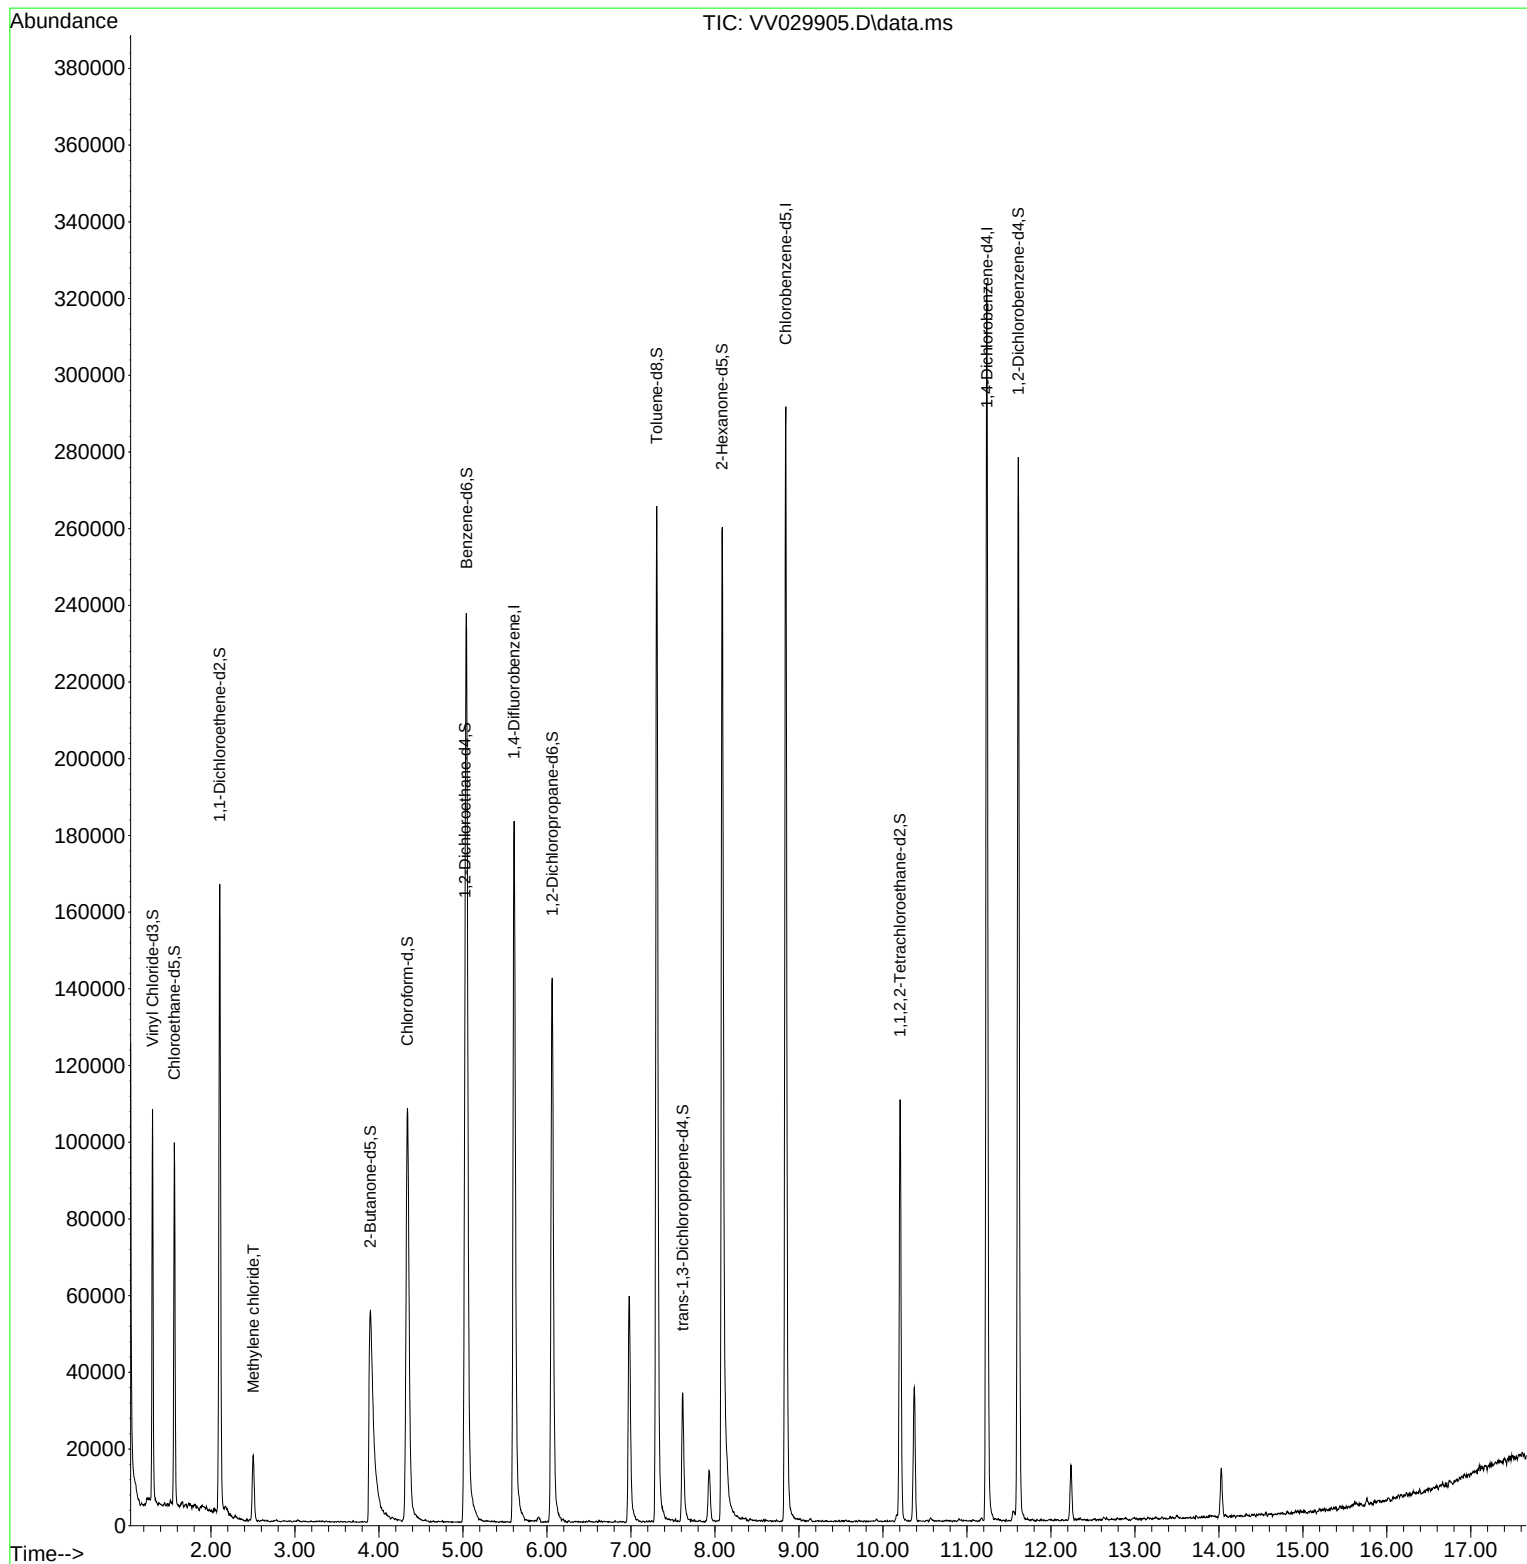

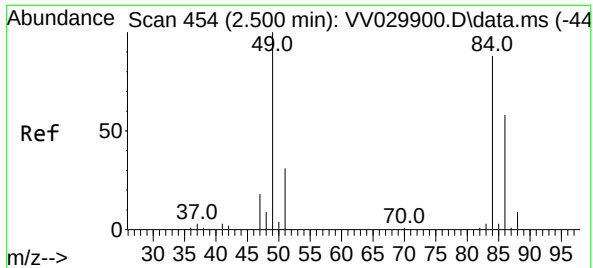

#16
Methylene chloride
Concen: 0.425 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV029905.D
Acq: 23 Jan 2023 16:05

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 7654
Ion Ratio Lower Upper
84 100
86 64.1 45.0 83.6
49 118.5 71.5 132.7

