

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012323\
 Data File : VW029917.D
 Acq On : 23 Jan 2023 20:54
 Operator : SY/MD
 Sample : 01225-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AG9

Quant Time: Jan 24 01:37:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 24 01:33:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	148164	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	149989	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	73197	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	61966	5.514	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	110.200%	
7) Chloroethane-d5	1.565	69	58494	6.279	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	125.600%	
11) 1,1-Dichloroethene-d2	2.105	63	81296	3.968	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	79.400%	
20) 2-Butanone-d5	3.915	46	107466	53.952	ug/L	0.03
Spiked Amount	50.000	Range 40 - 130	Recovery	=	107.900%	
24) Chloroform-d	4.339	84	112440	5.454	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	109.000%	
26) 1,2-Dichloroethane-d4	5.027	65	51430	5.891	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	117.800%	
32) Benzene-d6	5.043	84	212308	4.772	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.400%	
36) 1,2-Dichloropropane-d6	6.063	67	71480	5.490	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	109.800%	
41) Toluene-d8	7.307	98	170417	4.137	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	82.800%	
43) trans-1,3-Dichloroprop...	7.616	79	19770	4.157	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.200%	
46) 2-Hexanone-d5	8.088	63	100509	51.915	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	103.820%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	55935	5.862	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	117.200%	
66) 1,2-Dichlorobenzene-d4	11.612	152	65502	4.922	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.400%	
Target Compounds						Qvalue
34) Trichloroethene	5.915	95	1271	0.101	ug/L	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029917.D
Acq On : 23 Jan 2023 20:54
Operator : SY/MD
Sample : 01225-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AG9

Quant Time: Jan 24 01:37:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 24 01:33:02 2023
Response via : Initial Calibration

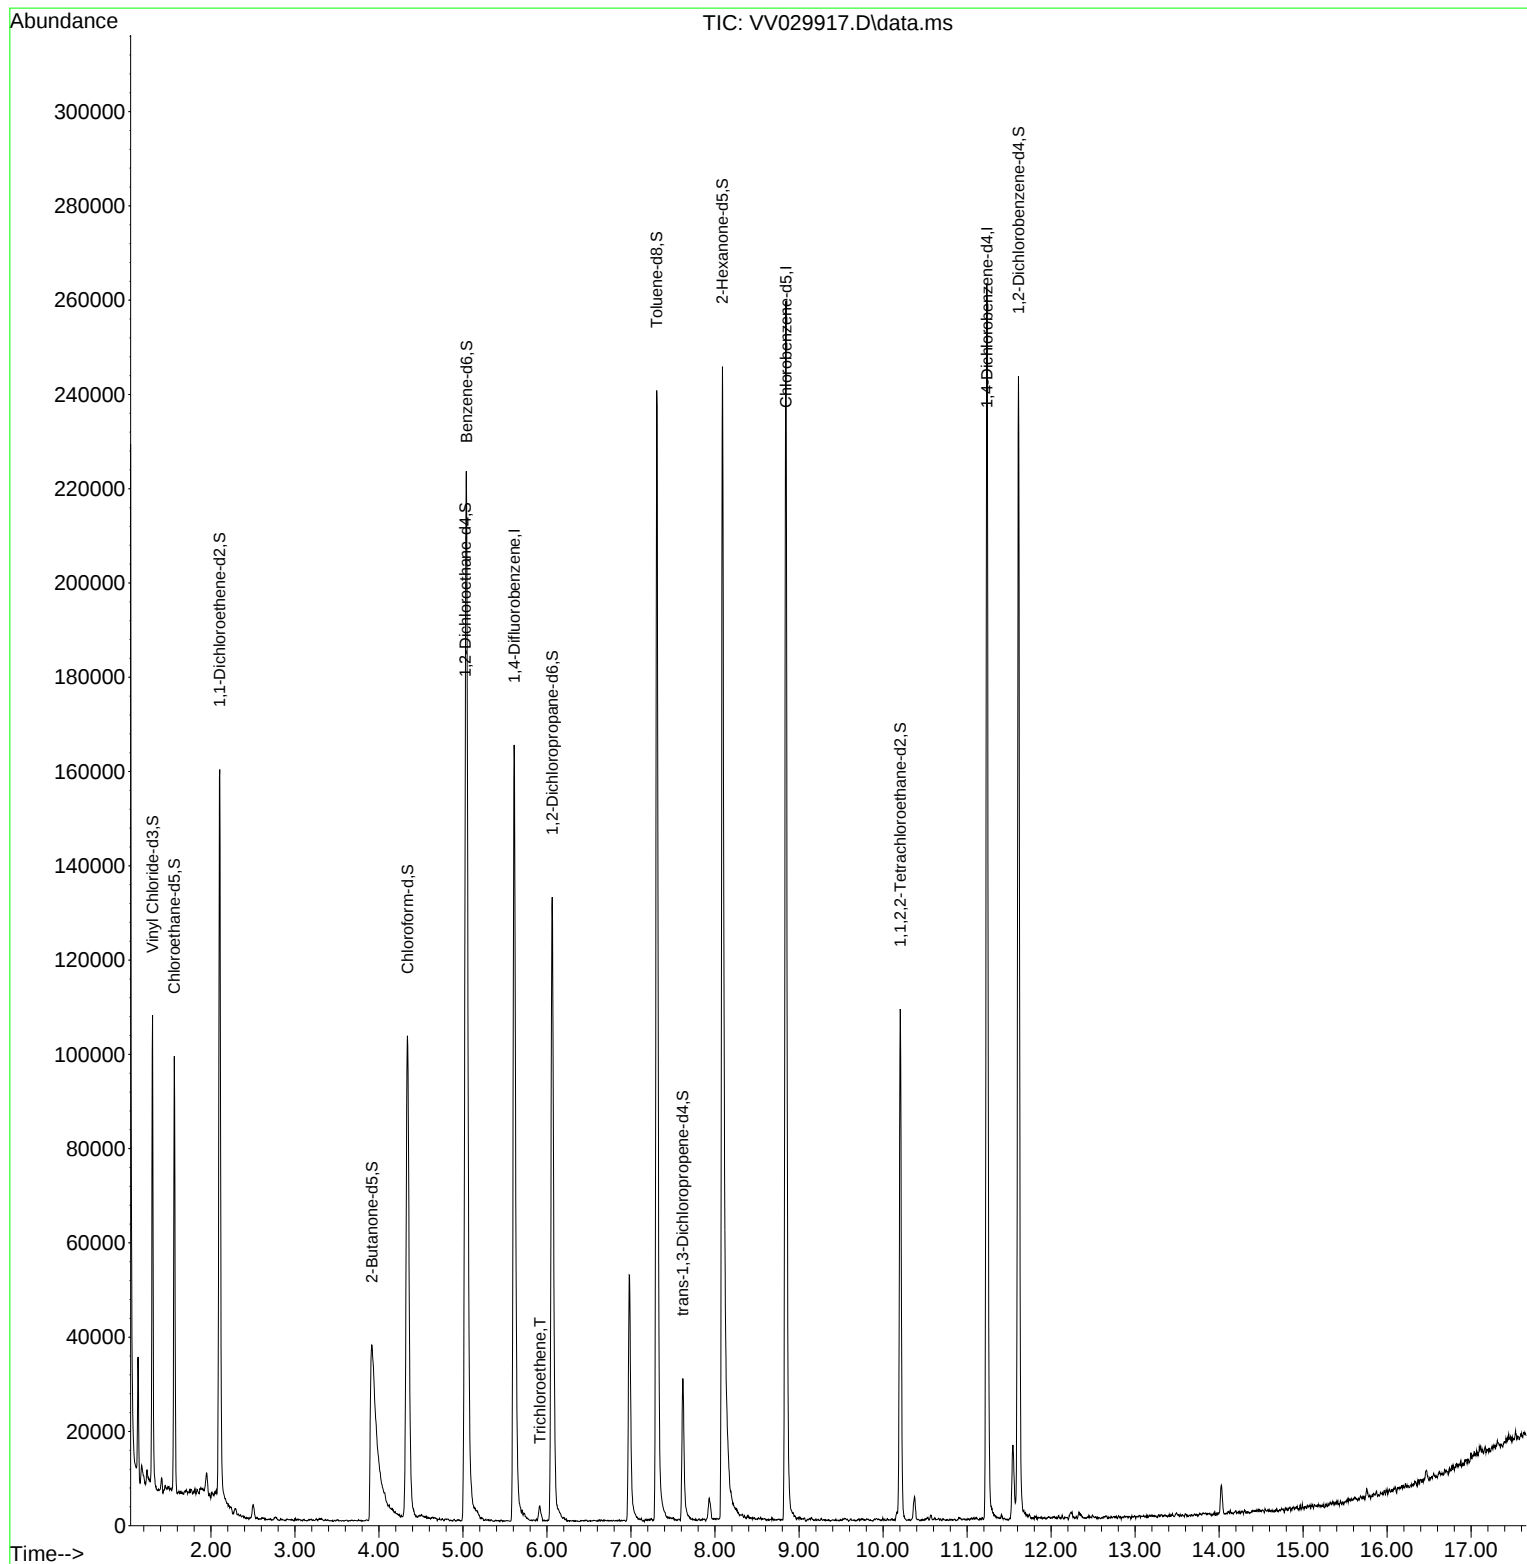

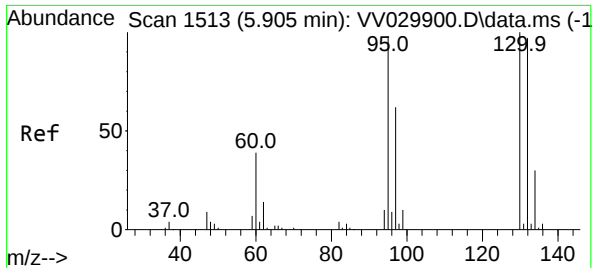

#34
 Trichloroethene
 Concen: 0.101 ug/L
 RT: 5.915 min Scan# 11
 Delta R.T. 0.010 min
 Lab File: VV029917.D
 Acq: 23 Jan 2023 20:54

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AG9

Tgt Ion: 95 Resp: 1271

Ion	Ratio	Lower	Upper
95	100		
97	52.5	44.9	83.3
132	87.0	71.8	133.4
130	71.5	75.3	139.8

