

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012323\
 Data File : VW029919.D
 Acq On : 23 Jan 2023 21:42
 Operator : SY/MD
 Sample : 01225-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9G8

Quant Time: Jan 24 01:37:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jan 24 01:33:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	157328	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	155724	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	79153	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	66796	5.598	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	112.000%
7) Chloroethane-d5	1.565	69	64396	6.510	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	130.200%#
11) 1,1-Dichloroethene-d2	2.105	63	88641	4.075	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.400%
20) 2-Butanone-d5	3.902	46	137938	65.217	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	130.440%#
24) Chloroform-d	4.339	84	124481	5.687	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.800%
26) 1,2-Dichloroethane-d4	5.024	65	54184	5.845	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.800%
32) Benzene-d6	5.043	84	232316	5.029	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.600%
36) 1,2-Dichloropropane-d6	6.063	67	78763	5.826	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	116.600%
41) Toluene-d8	7.307	98	185853	4.346	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.000%
43) trans-1,3-Dichloroprop...	7.616	79	20201	4.091	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.800%
46) 2-Hexanone-d5	8.088	63	110224	54.836	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.680%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	59999	6.056	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	121.200%#
66) 1,2-Dichlorobenzene-d4	11.612	152	71226	4.950	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.000%
Target Compounds						Qvalue
34) Trichloroethene	5.912	95	1258	0.096	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029919.D
Acq On : 23 Jan 2023 21:42
Operator : SY/MD
Sample : 01225-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9G8

Quant Time: Jan 24 01:37:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jan 24 01:33:02 2023
Response via : Initial Calibration

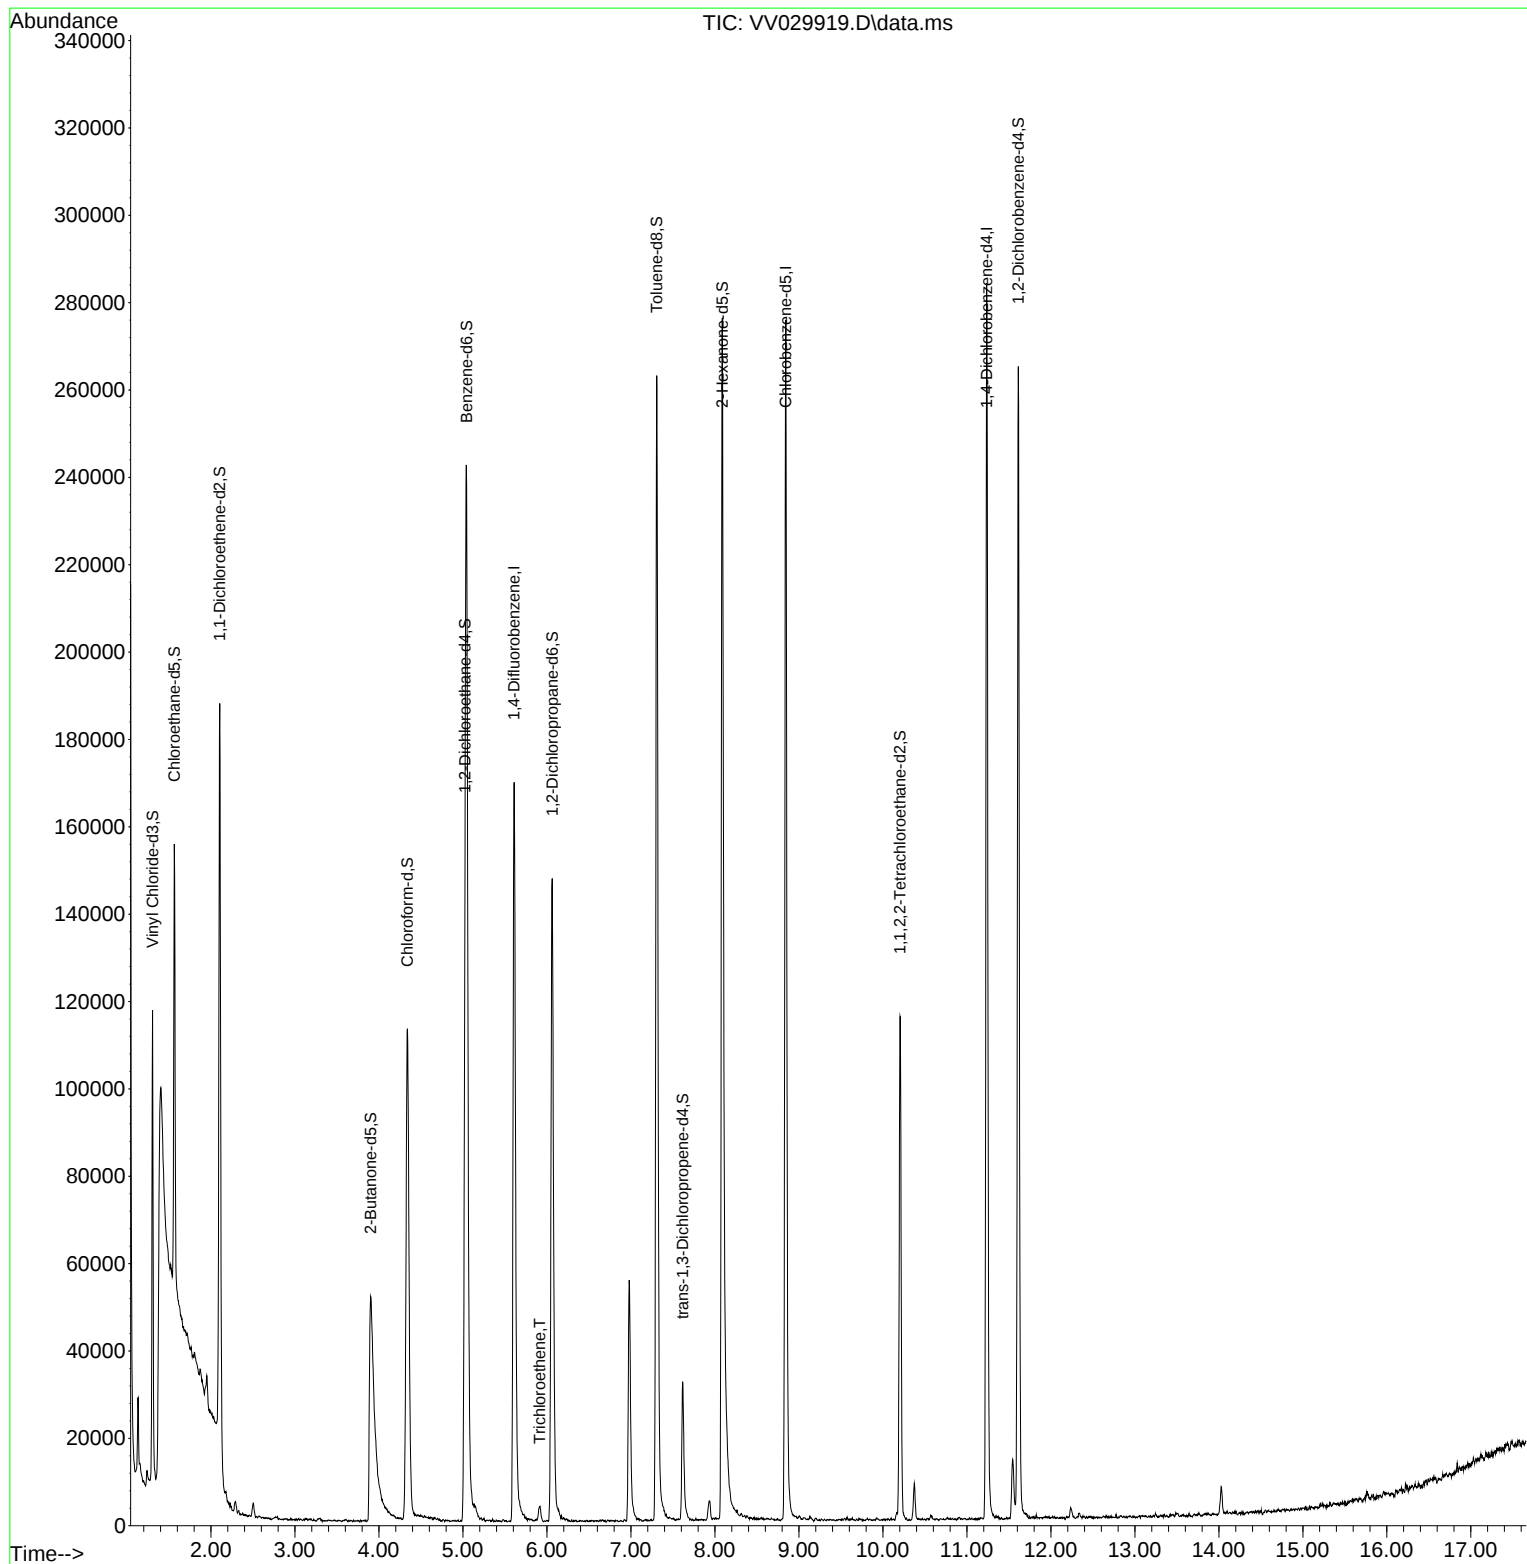

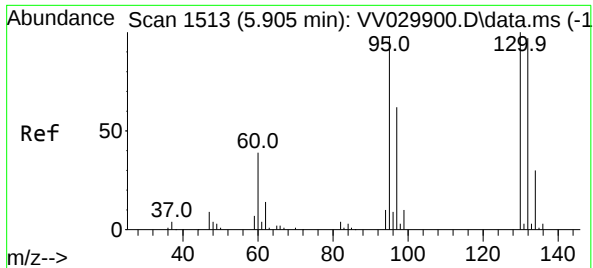

#34
 Trichloroethene
 Concen: 0.096 ug/L
 RT: 5.912 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VV029919.D
 Acq: 23 Jan 2023 21:42

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9G8

Tgt Ion: 95 Resp: 1258

Ion	Ratio	Lower	Upper
95	100		
97	59.3	44.9	83.3
132	105.7	71.8	133.4
130	104.9	75.3	139.8

