

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
 Data File : VV029901.D
 Acq On : 23 Jan 2023 13:45
 Operator : SY/MD
 Sample : VV0123WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK293

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	107030	107558	16.72%	2.007%
2	1.565	156	163	172	rBV	96710	107750	16.75%	2.010%
3	2.102	320	330	347	rBV	171032	247488	38.46%	4.618%
4	2.500	444	454	467	rBV2	27128	43660	6.79%	0.815%
5	3.892	872	887	926	rBV2	67643	267564	41.58%	4.992%
6	4.336	1008	1025	1047	rBV	110128	279635	43.46%	5.217%
7	5.037	1223	1243	1280	rBV2	246797	643453	100.00%	12.006%
8	5.606	1407	1420	1458	rBV	173473	372832	57.94%	6.956%
9	6.060	1544	1561	1590	rBV	145878	306059	47.57%	5.710%
10	6.976	1836	1846	1865	rBV	62035	118115	18.36%	2.204%
11	7.307	1935	1949	1981	rBV	283043	515542	80.12%	9.619%
12	7.613	2034	2044	2062	rBV	36042	66474	10.33%	1.240%
13	8.085	2179	2191	2231	rBV	274291	550632	85.57%	10.274%
14	8.413	2285	2293	2310	rVB3	4847	9207	1.43%	0.172%
15	8.841	2415	2426	2448	rBV	272354	469551	72.97%	8.761%
16	10.204	2840	2850	2867	rVB	111704	177110	27.52%	3.305%
17	10.371	2888	2902	2921	rVB	11121	19035	2.96%	0.355%
18	11.236	3160	3171	3191	rBV	326930	503633	78.27%	9.397%
19	11.612	3276	3288	3306	rBV	286546	462082	71.81%	8.622%
20	12.239	3472	3483	3494	rVB3	7257	13095	2.04%	0.244%
21	12.635	3597	3606	3617	rBV4	4545	7830	1.22%	0.146%
22	13.249	3789	3797	3806	rBV2	7663	11153	1.73%	0.208%
23	13.490	3861	3872	3887	rBV	17886	30846	4.79%	0.576%
24	13.731	3939	3947	3959	rBV3	7318	11819	1.84%	0.221%
25	14.030	4026	4040	4053	rBV2	10001	17493	2.72%	0.326%




Sum of corrected areas: 5359616

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029901.D
Acq On : 23 Jan 2023 13:45
Operator : SY/MD
Sample : VV0123WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK293

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

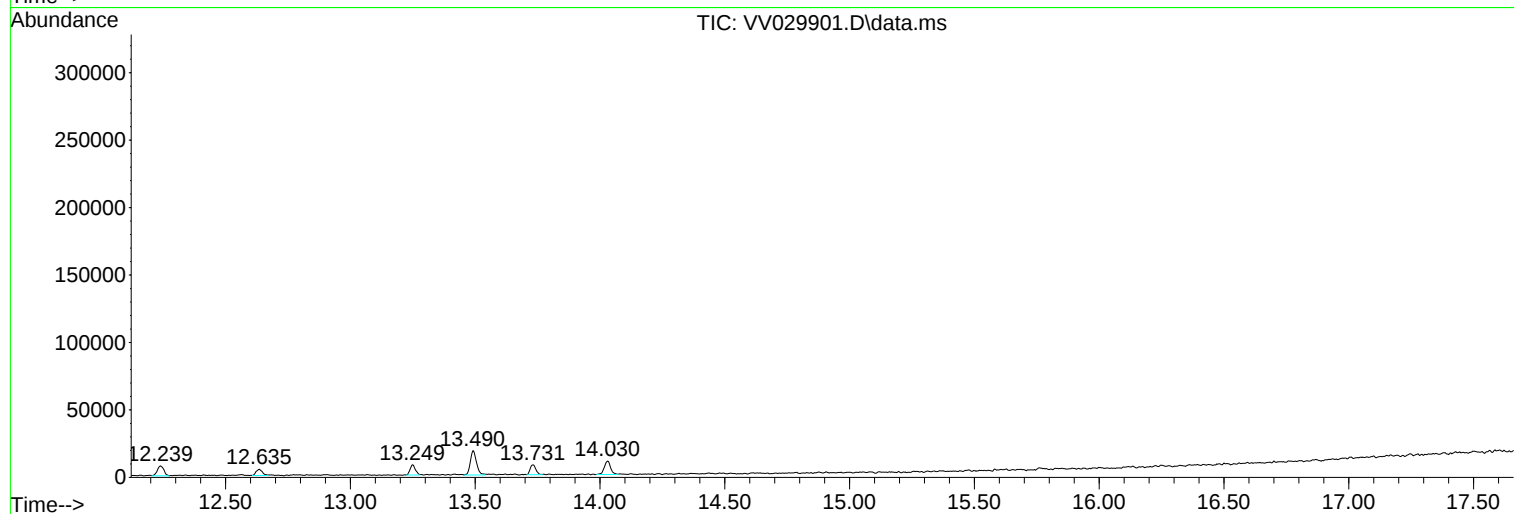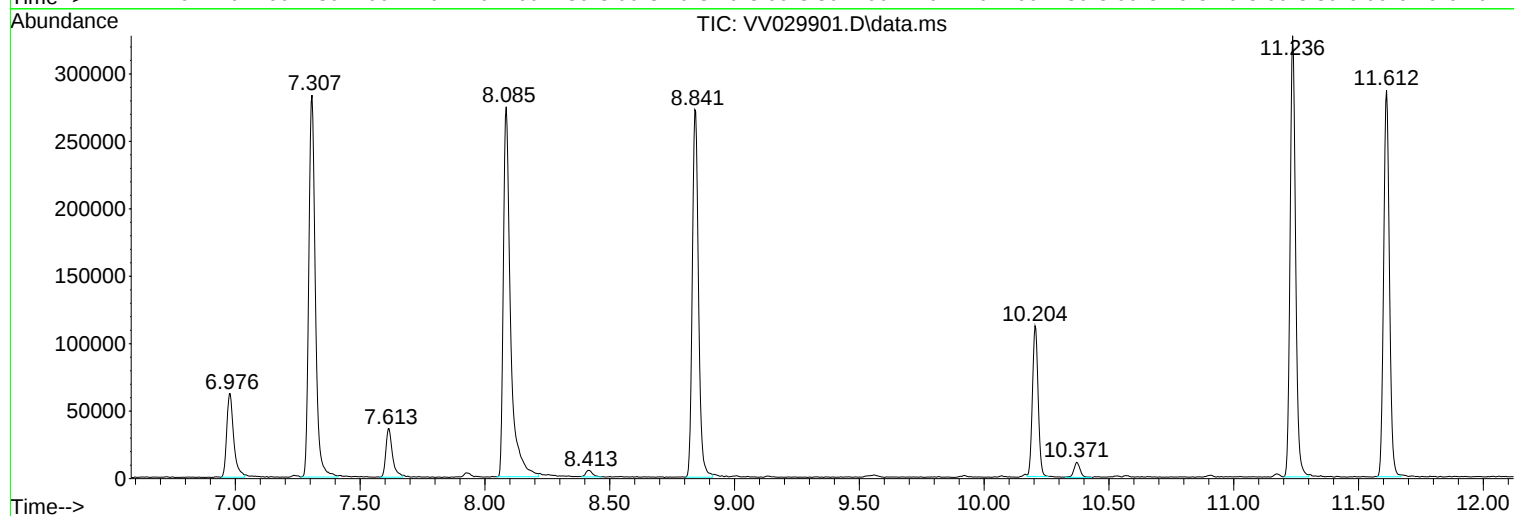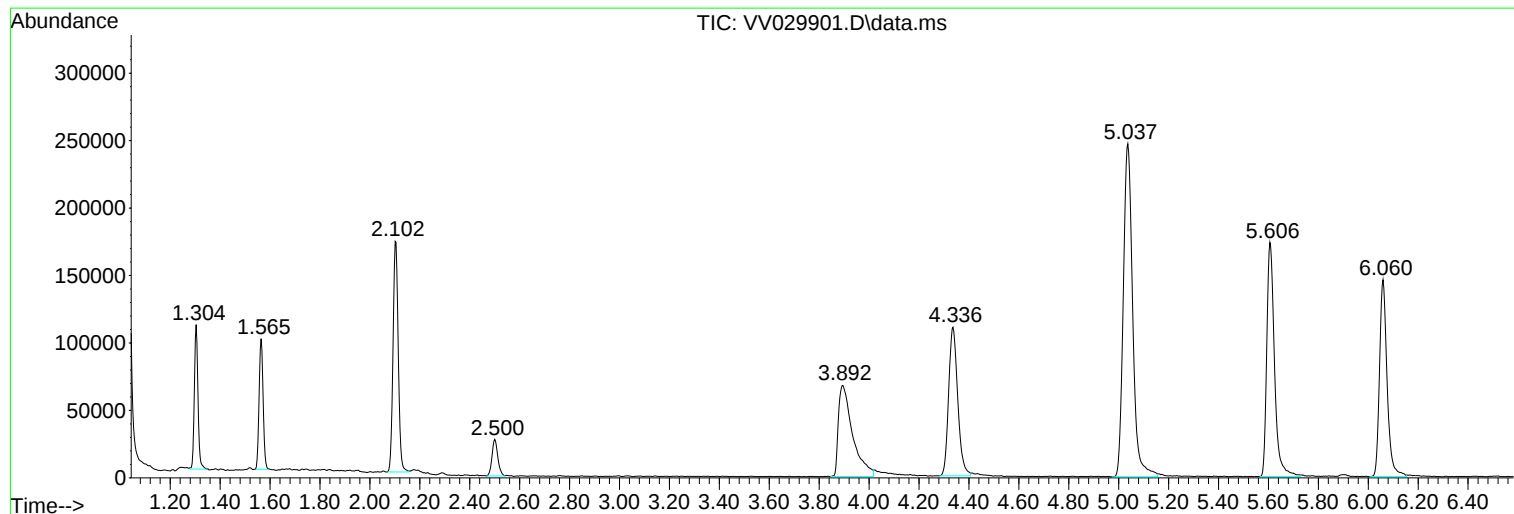

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029901.D
Acq On : 23 Jan 2023 13:45
Operator : SY/MD
Sample : VV0123WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK293

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029901.D
Acq On : 23 Jan 2023 13:45
Operator : SY/MD
Sample : VV0123WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK293

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc