

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
 Data File : VV029902.D
 Acq On : 23 Jan 2023 14:38
 Operator : SY/MD
 Sample : VV0123WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK294

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	106649	107404	17.22%	2.028%
2	1.564	156	163	175	rVB	97259	108720	17.43%	2.053%
3	2.105	319	331	345	rBV	167162	240349	38.54%	4.538%
4	2.500	443	454	468	rVB4	5086	8643	1.39%	0.163%
5	3.892	871	887	939	rBV2	62029	232230	37.23%	4.385%
6	4.339	1008	1026	1057	rBV2	111832	290913	46.64%	5.493%
7	5.040	1227	1244	1275	rBV2	242023	623705	100.00%	11.777%
8	5.609	1409	1421	1456	rBV	191842	403736	64.73%	7.623%
9	6.063	1546	1562	1591	rBV	144738	307277	49.27%	5.802%
10	6.979	1837	1847	1879	rBV	61103	117000	18.76%	2.209%
11	7.307	1937	1949	1973	rBV	276962	497708	79.80%	9.398%
12	7.616	2035	2045	2069	rBV	34770	66039	10.59%	1.247%
13	7.934	2132	2144	2152	rBV2	5792	10568	1.69%	0.200%
14	8.085	2180	2191	2230	rBV	270864	548617	87.96%	10.359%
15	8.844	2413	2427	2452	rBV	303857	506147	81.15%	9.557%
16	10.207	2840	2851	2866	rVB	114183	177554	28.47%	3.353%
17	10.374	2892	2903	2915	rVB	16949	27905	4.47%	0.527%
18	11.236	3160	3171	3190	rBV	334623	534620	85.72%	10.095%
19	11.612	3276	3288	3309	rVB	285456	453926	72.78%	8.571%
20	12.239	3475	3483	3492	rBV3	4175	6670	1.07%	0.126%
21	12.339	3504	3514	3524	rBV6	4303	6444	1.03%	0.122%
22	14.030	4030	4040	4050	rBV2	11625	19916	3.19%	0.376%




Sum of corrected areas: 5296091

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029902.D
Acq On : 23 Jan 2023 14:38
Operator : SY/MD
Sample : VV0123WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK294

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

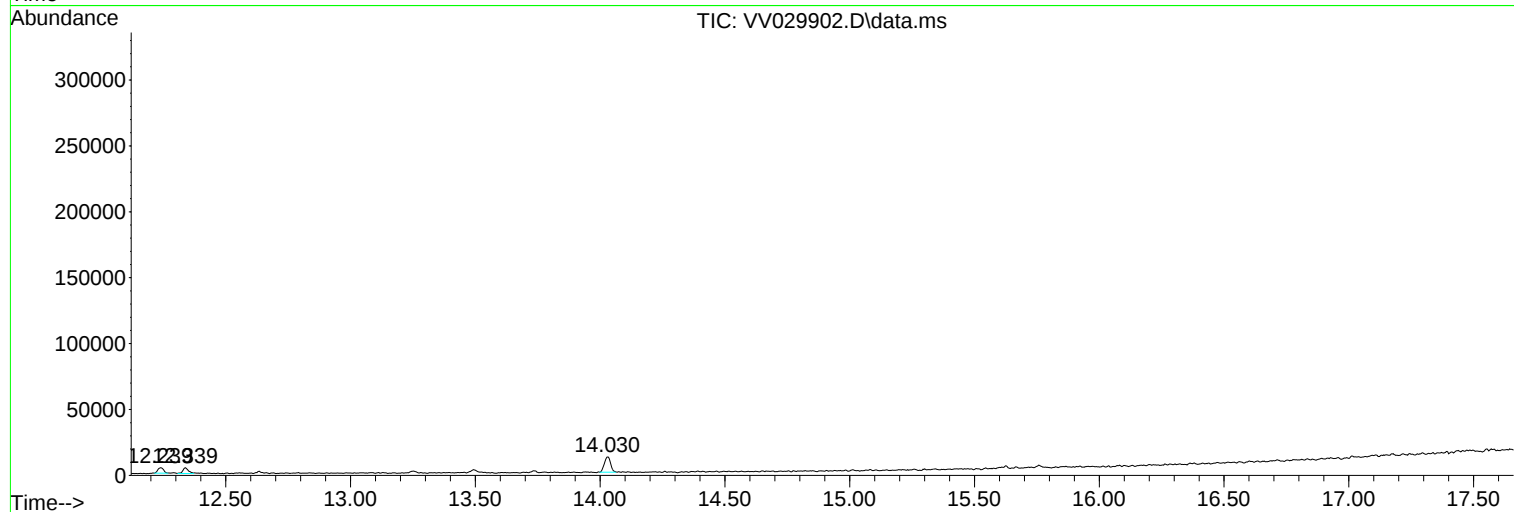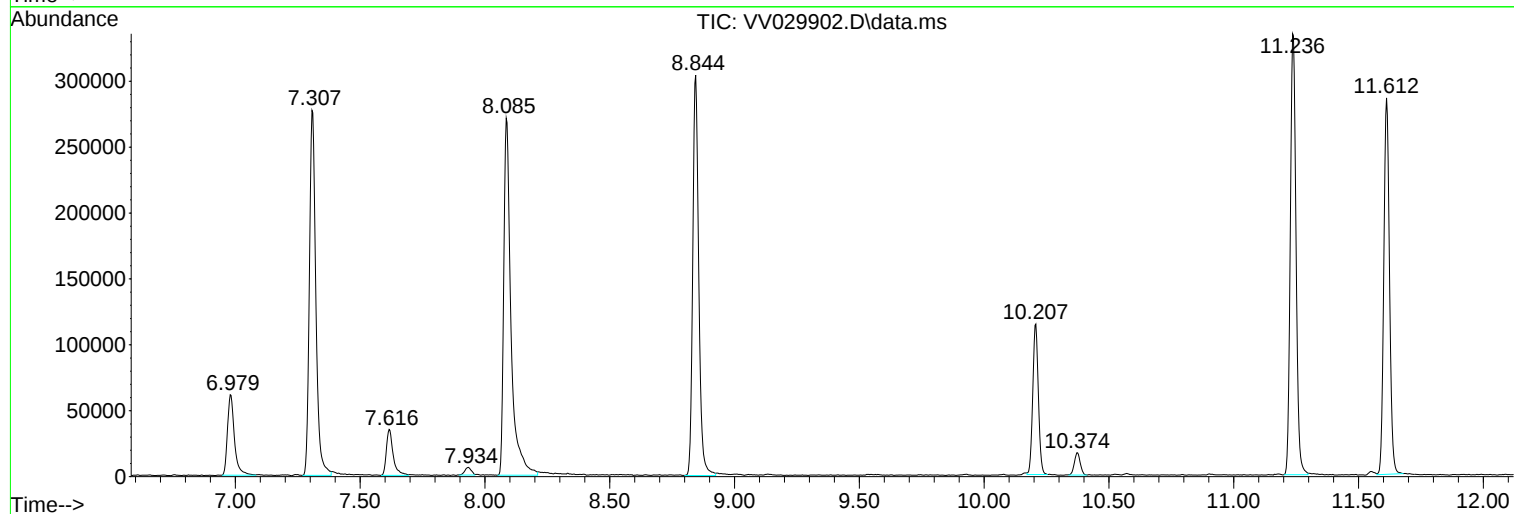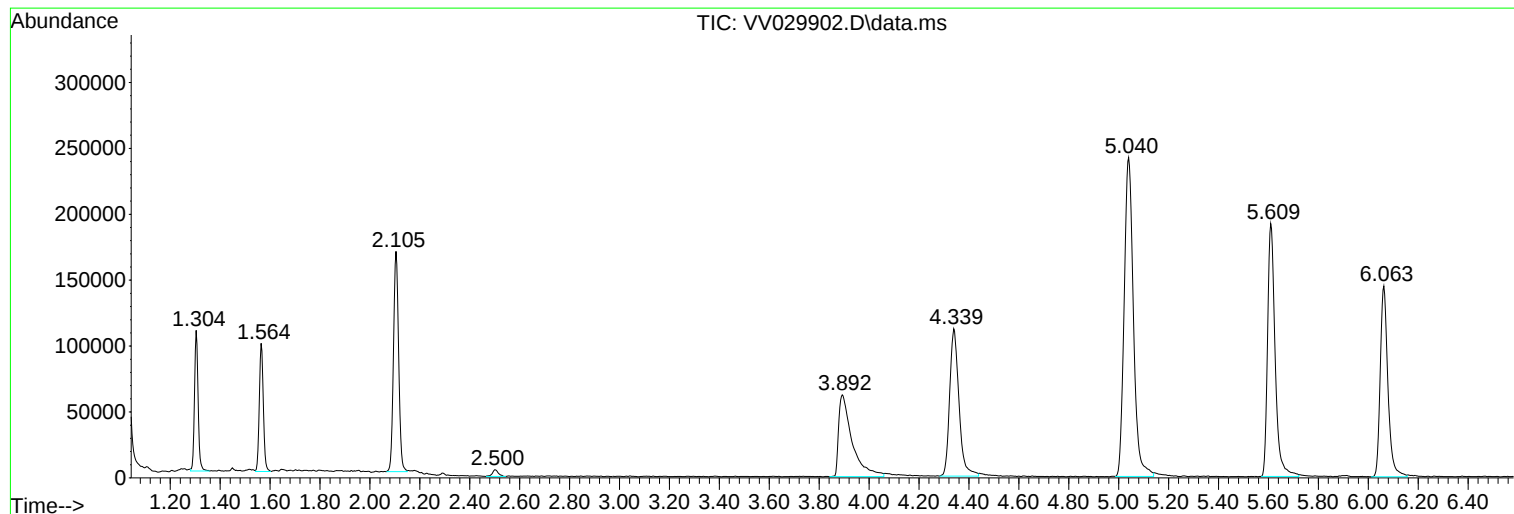

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029902.D
Acq On : 23 Jan 2023 14:38
Operator : SY/MD
Sample : VV0123WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK294

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029902.D
Acq On : 23 Jan 2023 14:38
Operator : SY/MD
Sample : VV0123WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK294

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc