

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
 Data File : VV029903.D
 Acq On : 23 Jan 2023 15:17
 Operator : SY/MD
 Sample : 01225-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9F2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	95713	95963	17.04%	1.952%
2	1.564	156	163	176	rVB	91624	101899	18.10%	2.072%
3	2.101	320	330	346	rBV	151751	219803	39.03%	4.470%
4	2.500	445	454	465	rVB4	4488	8131	1.44%	0.165%
5	3.889	874	886	942	rBV2	51927	189574	33.66%	3.856%
6	4.333	1008	1024	1057	rBV	98688	263988	46.88%	5.369%
7	5.037	1223	1243	1280	rBV2	217088	563120	100.00%	11.453%
8	5.606	1404	1420	1450	rBV	193038	407317	72.33%	8.284%
9	6.056	1547	1560	1590	rBV	129647	273634	48.59%	5.565%
10	6.976	1833	1846	1869	rBV2	56204	106171	18.85%	2.159%
11	7.304	1936	1948	1975	rBV	246126	445412	79.10%	9.059%
12	7.612	2035	2044	2060	rBV2	30486	55646	9.88%	1.132%
13	7.931	2129	2143	2159	rVB	15106	27815	4.94%	0.566%
14	8.085	2180	2191	2232	rBV	218582	448921	79.72%	9.130%
15	8.841	2413	2426	2455	rBV	297449	505786	89.82%	10.287%
16	10.204	2839	2850	2868	rVB	94865	152636	27.11%	3.104%
17	10.371	2891	2902	2917	rVB	51073	84931	15.08%	1.727%
18	11.236	3159	3171	3191	rBV	333965	531299	94.35%	10.805%
19	11.612	3276	3288	3304	rBV	244298	391850	69.59%	7.969%
20	12.239	3472	3483	3495	rVB2	14594	23149	4.11%	0.471%
21	14.030	4023	4040	4050	rBV	11224	19918	3.54%	0.405%




Sum of corrected areas: 4916963

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029903.D
Acq On : 23 Jan 2023 15:17
Operator : SY/MD
Sample : 01225-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9F2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

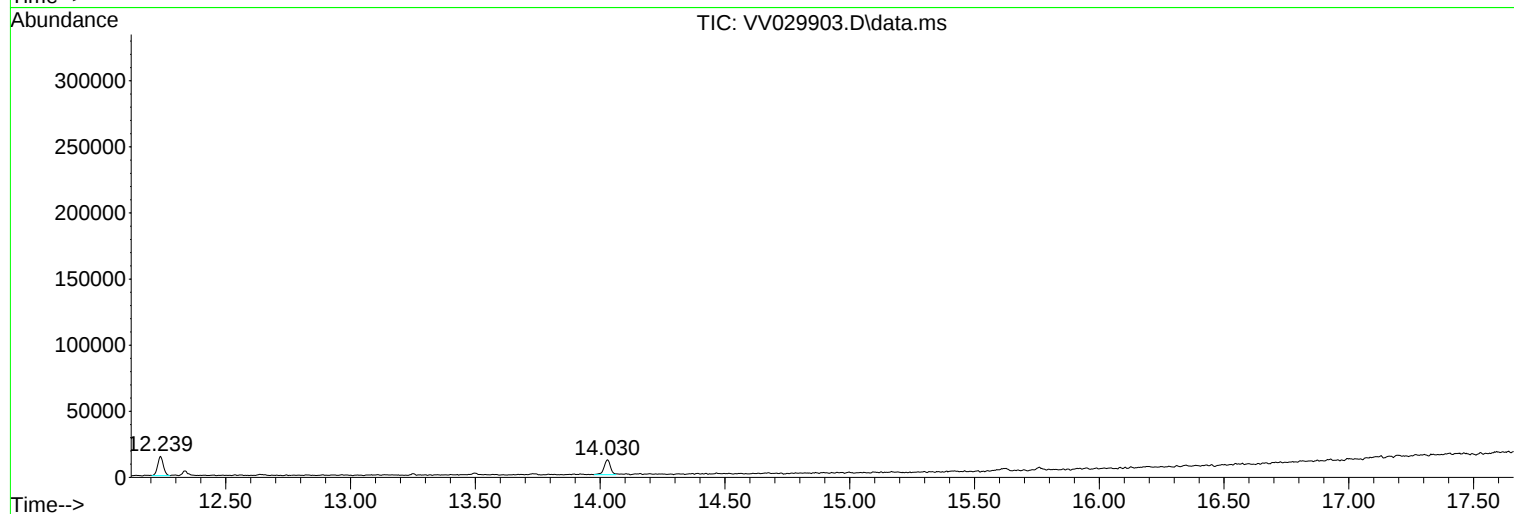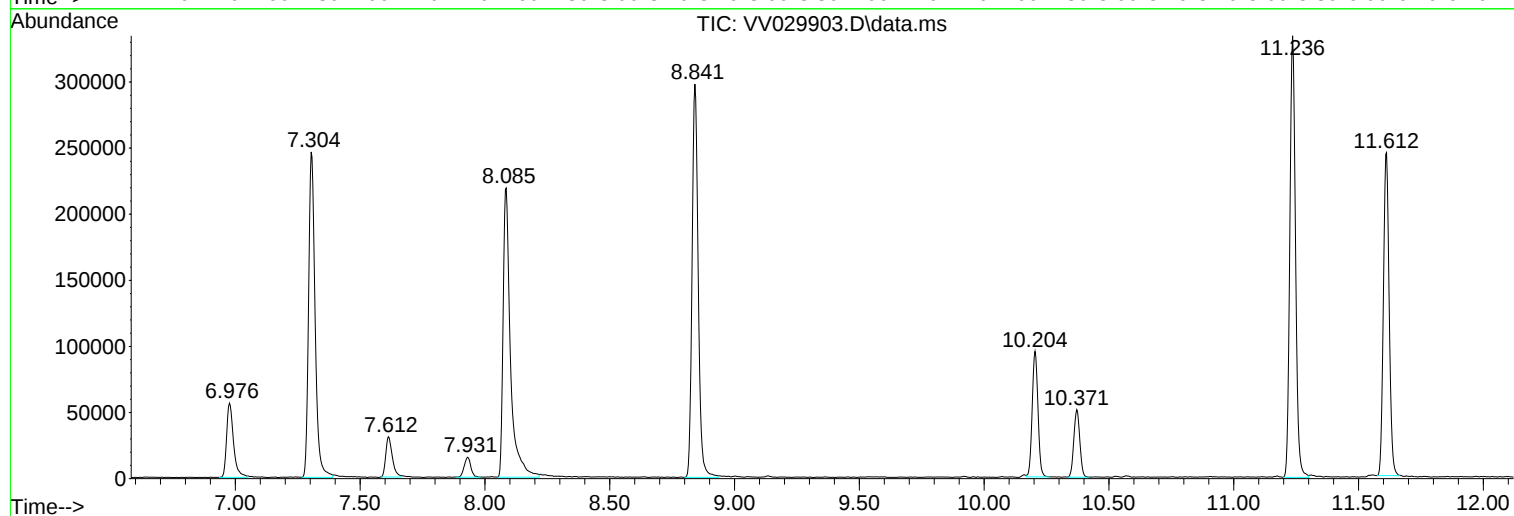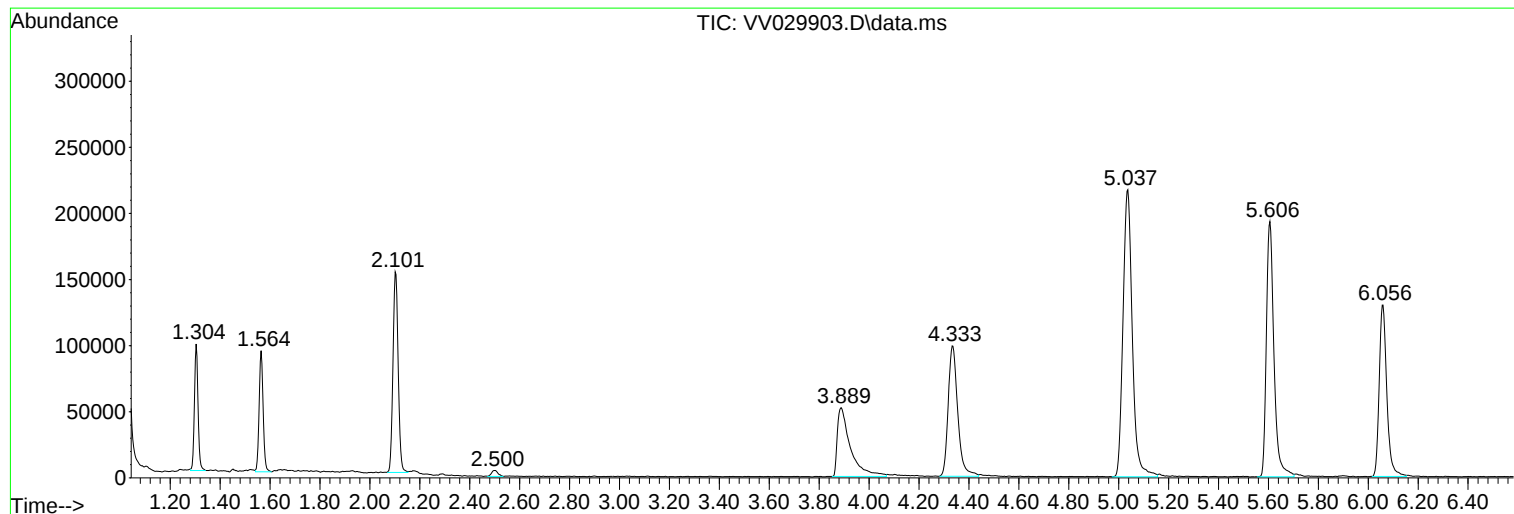

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029903.D
Acq On : 23 Jan 2023 15:17
Operator : SY/MD
Sample : 01225-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9F2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029903.D
Acq On : 23 Jan 2023 15:17
Operator : SY/MD
Sample : 01225-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9F2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------