

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
 Data File : VV029905.D
 Acq On : 23 Jan 2023 16:05
 Operator : SY/MD
 Sample : 01216-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029905.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	102462	102815	16.77%	1.982%
2	1.565	156	163	177	rVB	94763	105411	17.19%	2.032%
3	2.105	320	331	347	rBV	163660	237478	38.73%	4.579%
4	2.503	445	455	471	rVB	17140	29155	4.76%	0.562%
5	3.899	871	889	928	rBV	55417	212793	34.71%	4.103%
6	4.339	1006	1026	1053	rBV	107820	283031	46.16%	5.457%
7	5.040	1227	1244	1290	rBV2	236948	613114	100.00%	11.821%
8	5.609	1409	1421	1449	rBV	182783	382415	62.37%	7.373%
9	6.063	1548	1562	1592	rBV	141932	303374	49.48%	5.849%
10	6.979	1835	1847	1869	rBV	58989	112845	18.41%	2.176%
11	7.307	1936	1949	1974	rBV	264951	479033	78.13%	9.236%
12	7.616	2033	2045	2068	rBV	33636	63572	10.37%	1.226%
13	7.931	2132	2143	2158	rVB2	13127	24884	4.06%	0.480%
14	8.088	2179	2192	2232	rBV	259105	532505	86.85%	10.267%
15	8.844	2415	2427	2444	rBV	290505	482870	78.76%	9.310%
16	10.204	2840	2850	2867	rVB	109605	171740	28.01%	3.311%
17	10.374	2887	2903	2915	rBV	34915	58665	9.57%	1.131%
18	11.236	3160	3171	3190	rBV	322614	508335	82.91%	9.801%
19	11.612	3276	3288	3312	rVB	276884	436957	71.27%	8.425%
20	12.239	3470	3483	3495	rBV2	14485	23375	3.81%	0.451%
21	14.030	4027	4040	4050	rBV	12911	22169	3.62%	0.427%




Sum of corrected areas: 5186536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029905.D
Acq On : 23 Jan 2023 16:05
Operator : SY/MD
Sample : 01216-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

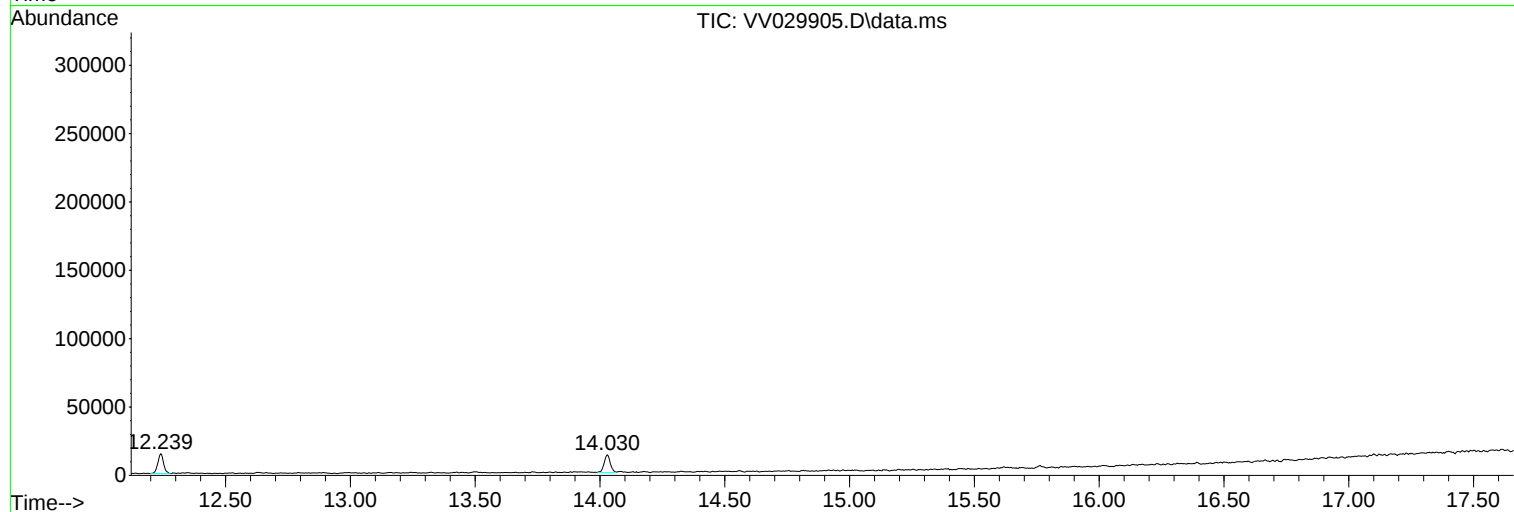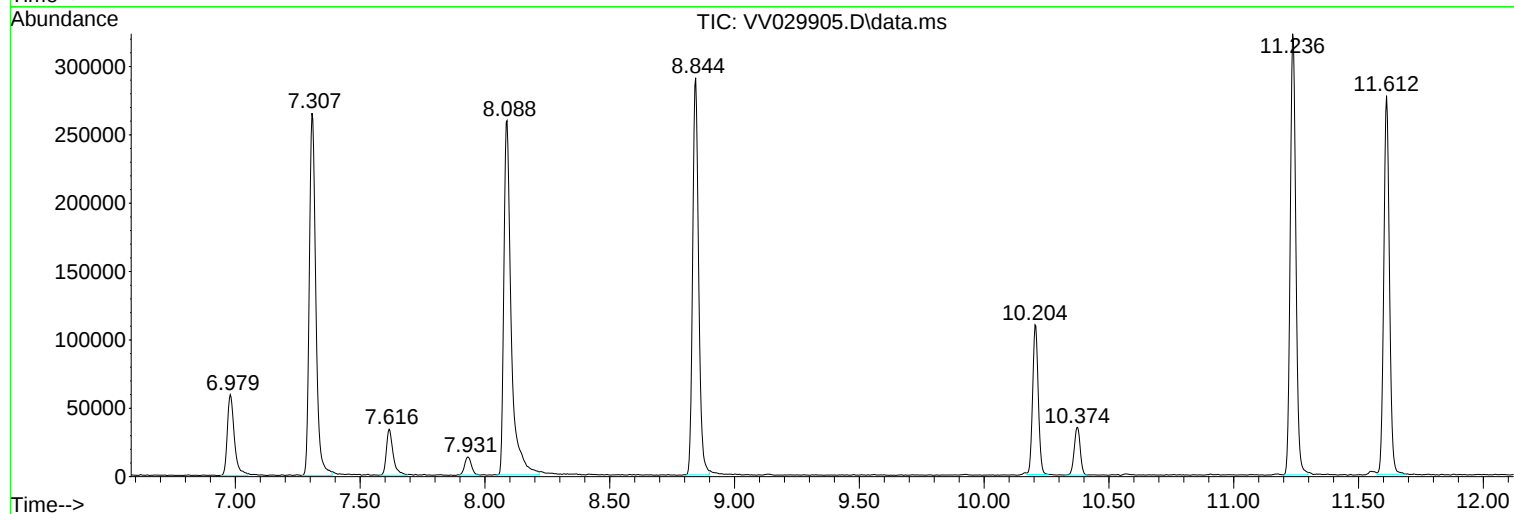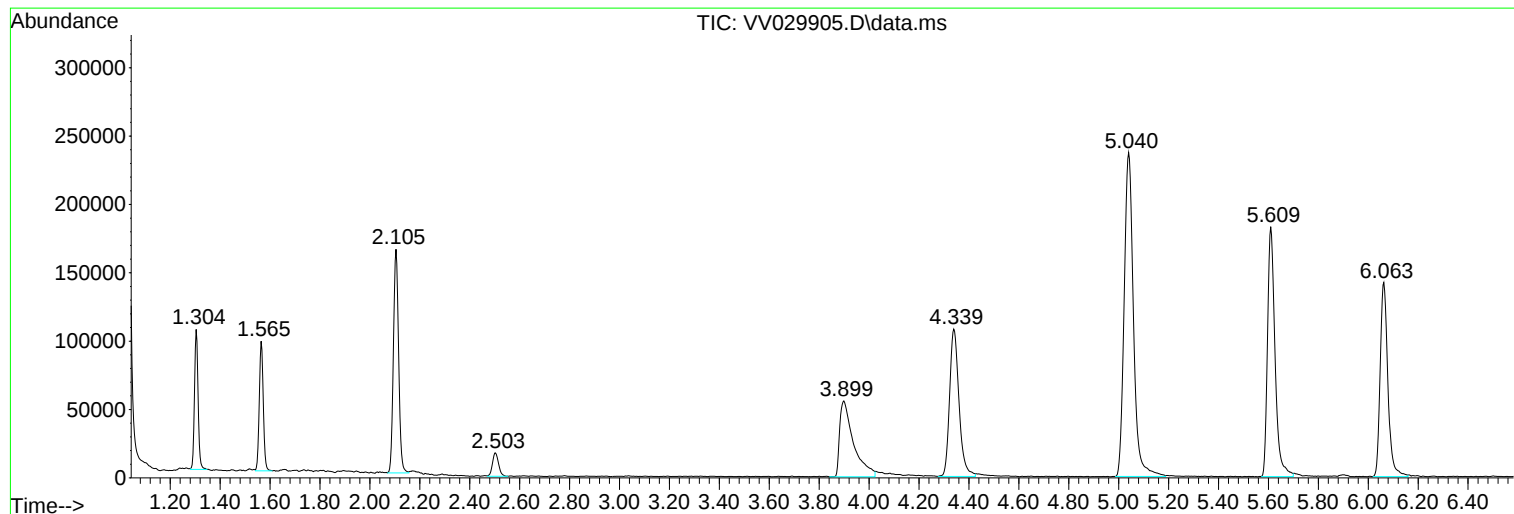

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029905.D
Acq On : 23 Jan 2023 16:05
Operator : SY/MD
Sample : 01216-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029905.D
Acq On : 23 Jan 2023 16:05
Operator : SY/MD
Sample : 01216-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc