

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
 Data File : VV029911.D
 Acq On : 23 Jan 2023 18:30
 Operator : SY/MD
 Sample : 01225-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9F5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	25	rVV2	8538	8194	1.39%	0.159%
2	1.130	25	28	37	rVB	20038	19805	3.36%	0.385%
3	1.214	49	54	60	rBV	23063	20869	3.54%	0.406%
4	1.304	75	82	89	rBV	94363	94295	15.98%	1.834%
5	1.413	109	116	122	rBV	22044	24067	4.08%	0.468%
6	1.565	156	163	172	rVB	89502	98270	16.66%	1.912%
7	1.944	276	281	291	rVB3	6796	9106	1.54%	0.177%
8	2.105	321	331	345	rVB	151993	216317	36.67%	4.208%
9	2.761	526	535	544	rBV3	5694	10359	1.76%	0.202%
10	3.188	656	668	680	rBV3	4296	8527	1.45%	0.166%
11	3.899	876	889	933	rBV3	97636	330914	56.09%	6.438%
12	4.339	1009	1026	1050	rBV	103082	261671	44.36%	5.091%
13	5.040	1227	1244	1281	rBV2	224768	589920	100.00%	11.477%
14	5.609	1407	1421	1448	rBV	181213	384763	65.22%	7.485%
15	6.063	1544	1562	1591	rBV	137484	293999	49.84%	5.720%
16	6.979	1837	1847	1869	rBV	54302	105925	17.96%	2.061%
17	7.307	1935	1949	1977	rBV	249670	453826	76.93%	8.829%
18	7.616	2033	2045	2066	rBV2	32488	60937	10.33%	1.185%
19	7.931	2131	2143	2156	rBV2	9021	16820	2.85%	0.327%
20	8.085	2181	2191	2228	rBV	256639	524904	88.98%	10.212%
21	8.844	2412	2427	2446	rBV	286642	480387	81.43%	9.346%
22	10.204	2840	2850	2869	rVB	105298	168416	28.55%	3.276%
23	10.374	2891	2903	2914	rBV2	23799	40073	6.79%	0.780%
24	11.236	3160	3171	3192	rBV	307515	480813	81.50%	9.354%
25	11.612	3277	3288	3310	rVB	255617	410685	69.62%	7.990%
26	12.239	3472	3483	3493	rBV2	6938	11095	1.88%	0.216%
27	14.030	4030	4040	4055	rVB2	9264	15272	2.59%	0.297%




Sum of corrected areas: 5140229

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029911.D
Acq On : 23 Jan 2023 18:30
Operator : SY/MD
Sample : 01225-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9F5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

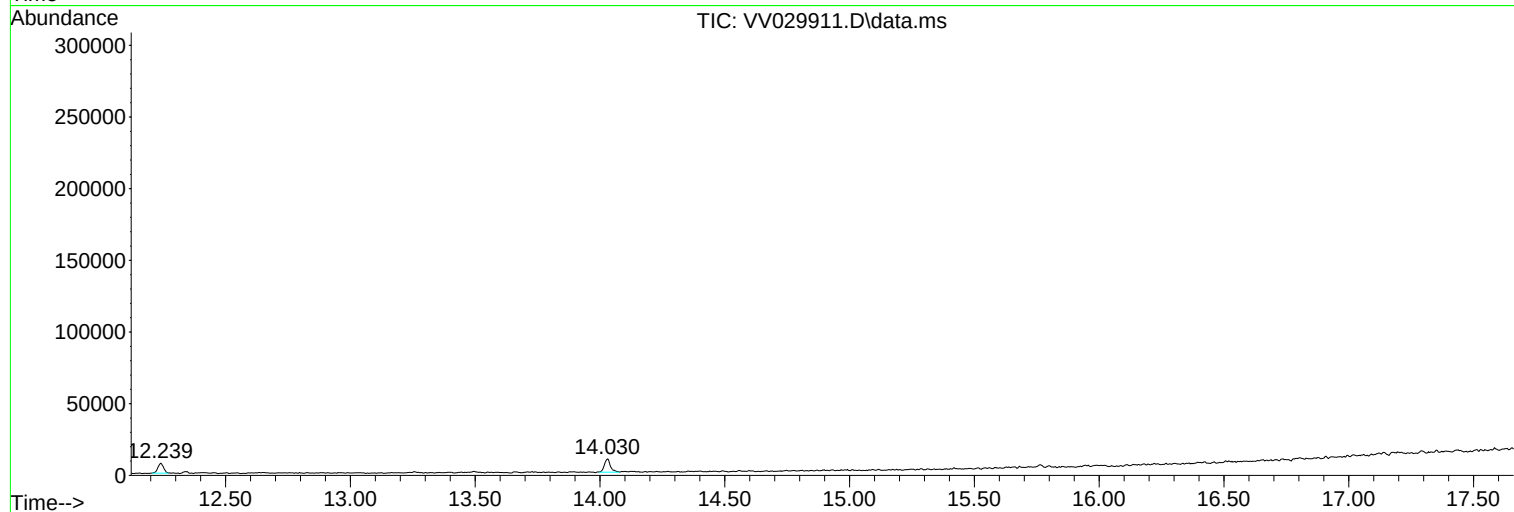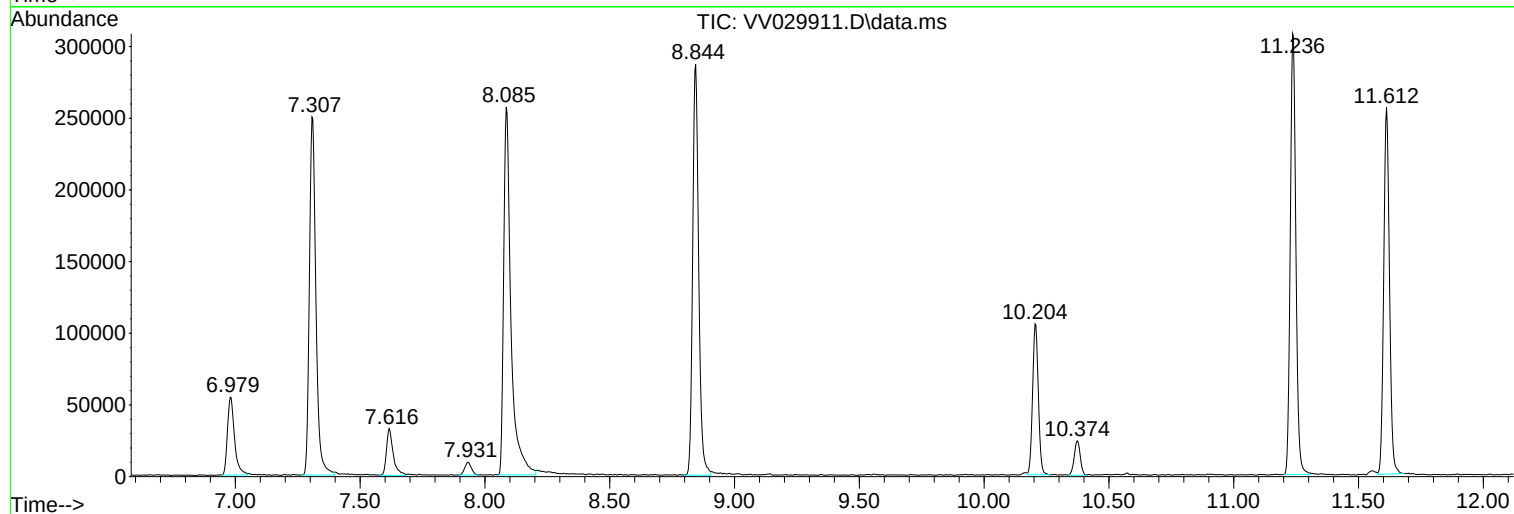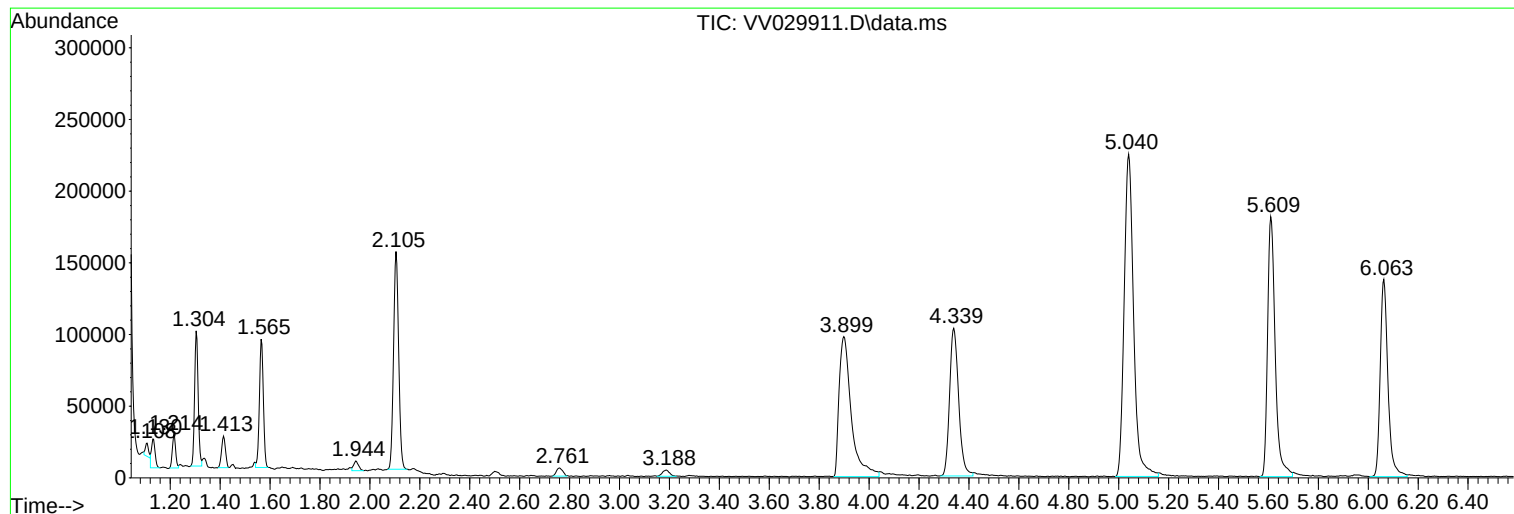

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029911.D
Acq On : 23 Jan 2023 18:30
Operator : SY/MD
Sample : 01225-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9F5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
Data File : VV029911.D
Acq On : 23 Jan 2023 18:30
Operator : SY/MD
Sample : 01225-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9F5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------