


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012323\
 Data File : VV029899.D
 Acq On : 23 Jan 2023 12:20
 Operator : SY/MD
 Sample : BFB214
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB214

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jan 25 22:12:17 2023

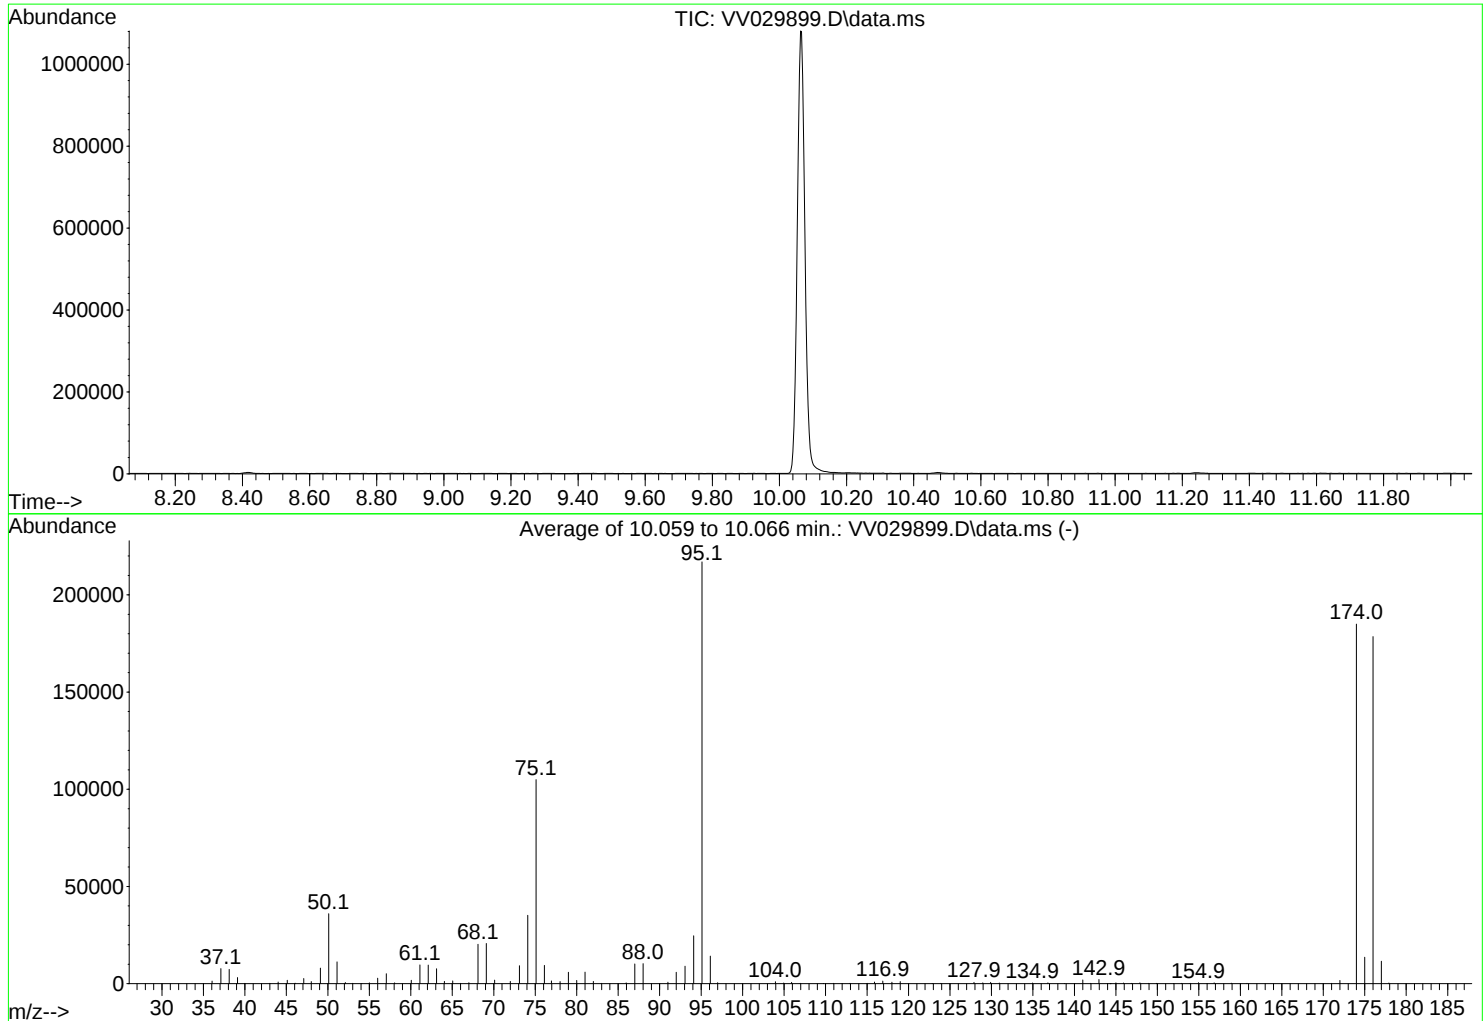

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	35957	PASS
75	95	30	80	48.4	104915	PASS
95	95	100	100	100.0	216981	PASS
96	95	5	9	6.5	14124	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.3	184981	PASS
175	174	5	9	7.3	13578	PASS
176	174	95	105	96.5	178496	PASS
177	176	5	10	6.4	11504	PASS

m/z	Abundance
40.00	314.0
44.00	866.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
36.00	1310.0
37.10	7492.0
38.10	7031.0
39.10	3070.0
40.00	489.0
43.00	157.0
44.00	1617.0
45.10	1667.0
46.20	219.0
47.10	2374.0
48.00	1033.0
49.10	7703.0
50.10	34528.0
51.10	10517.0
52.10	570.0
53.00	149.0
54.10	108.0
55.00	412.0
56.00	2812.0
57.00	4954.0
58.00	371.0
60.10	1631.0
61.10	9218.0
62.10	9032.0
63.10	7177.0
64.00	1140.0
65.10	1311.0
66.00	220.0
67.00	464.0
68.10	19096.0
69.10	19424.0
70.10	1624.0
72.00	1198.0
73.10	8802.0
74.10	32936.0
75.10	99000.0
76.10	8999.0
76.90	1342.0
78.00	994.0
79.00	5539.0
80.00	1526.0
81.00	5680.0
82.00	987.0
83.00	175.0
85.90	382.0
87.00	9705.0
88.00	9638.0
91.00	772.0
92.00	5442.0
93.00	8619.0
94.10	22864.0
95.10	203712.0
96.10	14077.0
97.00	484.0
104.00	1001.0
105.00	294.0
105.90	695.0
106.90	188.0
109.80	104.0
110.90	180.0
113.00	210.0
115.00	205.0
115.90	771.0
116.90	1232.0
118.00	774.0
119.00	1016.0
122.90	112.0
123.90	167.0
127.90	609.0
129.00	369.0
129.90	656.0
131.00	279.0
134.90	318.0
136.80	352.0
140.10	109.0
141.00	1707.0
142.10	182.0
142.90	1982.0
144.30	131.0
145.00	459.0
145.90	359.0
146.80	141.0
147.90	406.0
149.00	106.0
149.90	177.0
152.00	113.0
152.90	128.0
154.00	108.0
155.00	521.0
156.00	129.0
156.80	406.0
158.90	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

160.80	179.0
171.00	189.0
172.00	1613.0
174.00	169344.0
175.00	12919.0
176.00	163264.0
177.00	10817.0
177.90	312.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
36.10	1371.0
37.10	7906.0
38.10	7624.0
39.10	3259.0
40.00	538.0
43.00	208.0
44.00	1746.0
45.10	1753.0
46.00	221.0
47.10	2834.0
48.00	1146.0
49.10	8297.0
50.10	37216.0
51.10	11586.0
52.10	594.0
53.00	163.0
54.10	102.0
55.00	461.0
56.00	2915.0
57.00	5288.0
58.00	422.0
60.00	1774.0
61.10	10030.0
62.10	9879.0
63.10	7994.0
64.00	1205.0
65.00	1440.0
66.00	178.0
67.00	544.0
68.10	20904.0
69.10	21288.0
70.10	1859.0
72.00	1260.0
73.10	9514.0
74.10	36320.0
75.10	108264.0
76.10	9715.0
76.90	1462.0
78.00	1106.0
79.00	6106.0
80.00	1685.0
81.00	6141.0
82.00	1155.0
83.00	199.0
86.00	462.0
87.00	10477.0
88.00	10521.0
91.00	820.0
92.00	6062.0
93.00	9305.0
94.10	25496.0
95.10	224768.0
96.10	14521.0
97.00	493.0
104.00	988.0
104.90	331.0
105.90	713.0
106.90	192.0
109.70	130.0
111.00	181.0
112.00	116.0
113.00	211.0
115.00	220.0
115.90	820.0
116.90	1365.0
118.00	829.0
119.00	1134.0
122.80	111.0
123.90	171.0
127.90	719.0
128.90	472.0
129.90	655.0
130.90	292.0
135.00	351.0
136.80	392.0
138.80	106.0
140.10	110.0
141.00	2030.0
141.90	184.0
142.90	2266.0
144.00	133.0
145.00	453.0
145.90	349.0
146.90	188.0
147.90	442.0
149.00	131.0
149.90	204.0
151.90	117.0
152.90	154.0
153.90	150.0
154.90	549.0
156.00	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

156.90	453.0
158.90	253.0
160.80	205.0
171.00	181.0
172.00	1633.0
174.00	191040.0
175.00	13974.0
176.00	184384.0
177.00	11863.0
177.90	336.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
36.10	1380.0
37.10	7770.0
38.10	7369.0
39.10	3158.0
40.00	520.0
43.00	226.0
44.00	1783.0
45.10	1671.0
46.00	259.0
47.10	2802.0
48.00	1131.0
49.10	8019.0
50.10	36128.0
51.10	11455.0
52.10	557.0
53.00	163.0
55.00	458.0
56.00	2745.0
57.10	5172.0
58.10	372.0
60.00	1870.0
61.10	9768.0
62.10	9777.0
63.10	7824.0
64.10	1044.0
65.00	1400.0
66.00	145.0
67.00	520.0
68.10	20720.0
69.10	21392.0
70.10	1849.0
72.00	1107.0
73.10	9364.0
74.10	36304.0
75.10	107480.0
76.10	9388.0
77.00	1434.0
78.00	1055.0
79.00	6008.0
80.00	1676.0
81.00	5988.0
82.00	1255.0
82.90	190.0
86.00	506.0
87.00	10318.0
88.00	10699.0
91.00	761.0
92.00	6139.0
93.10	9077.0
94.10	25560.0
95.10	222464.0
96.10	13774.0
97.00	430.0
103.90	895.0
104.90	346.0
105.90	697.0
107.00	189.0
109.70	147.0
110.90	188.0
112.00	187.0
112.90	196.0
115.00	208.0
115.90	805.0
116.90	1319.0
118.00	755.0
119.00	1121.0
122.80	101.0
123.90	151.0
127.90	767.0
128.90	459.0
129.90	606.0
130.90	320.0
135.00	338.0
136.80	398.0
138.80	103.0
140.00	112.0
141.00	2037.0
141.90	193.0
143.00	2267.0
144.00	148.0
145.00	389.0
145.90	326.0
146.90	228.0
147.90	464.0
148.90	152.0
149.90	220.0
151.90	121.0
152.90	179.0
153.90	172.0
154.90	548.0
156.90	429.0
158.90	280.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

160.80	234.0
171.00	149.0
172.00	1612.0
174.00	194560.0
175.00	13842.0
176.00	187840.0
177.00	11833.0
177.90	322.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214