
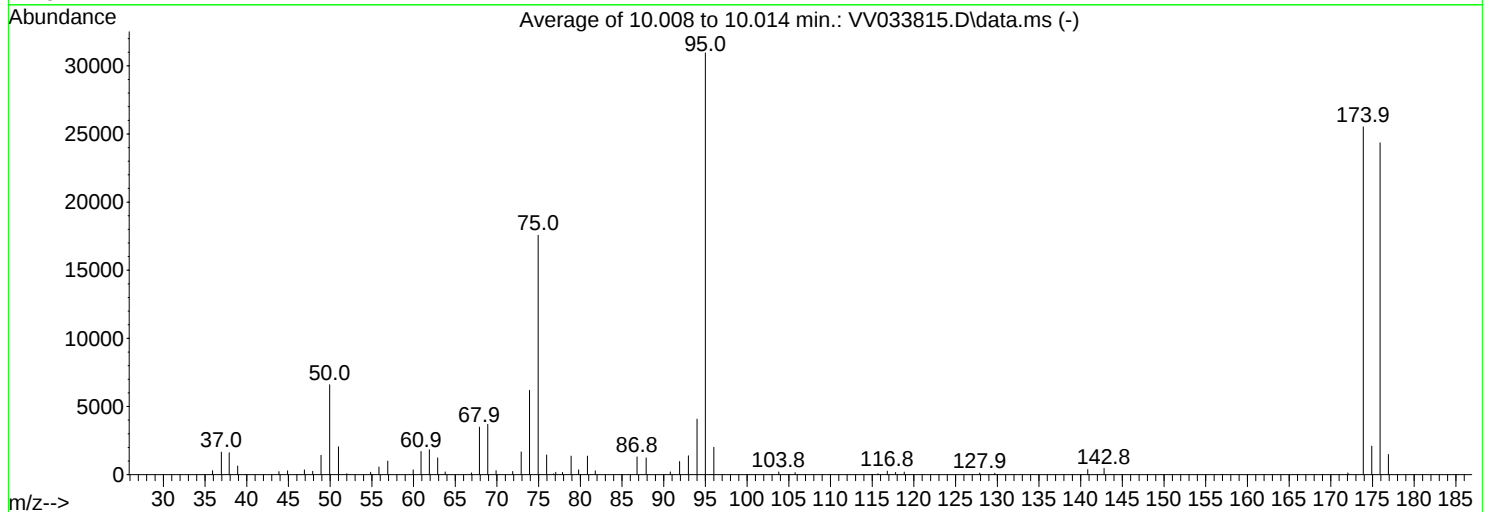


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012324\
Data File : VV033815.D
Acq On : 23 Jan 2024 08:41
Operator : SY/MD
Sample : BFB256
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB256

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Title : VOC Analysis
Last Update : Wed Jan 24 02:00:55 2024

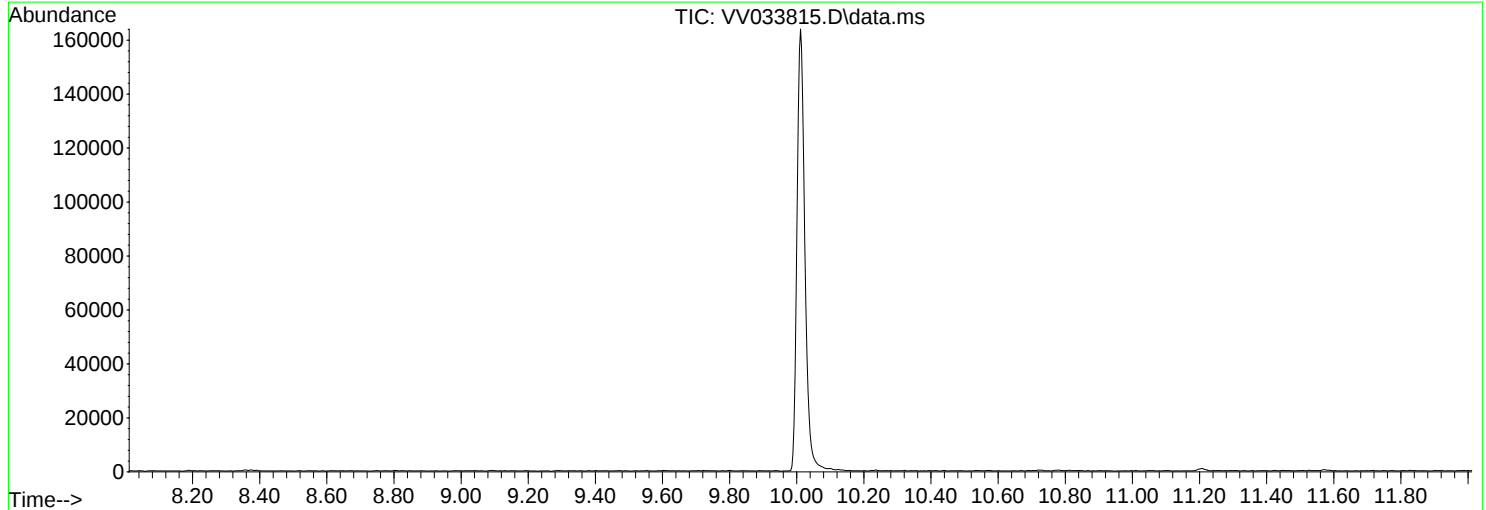

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.3	6598	PASS
75	95	30	80	56.7	17563	PASS
95	95	100	100	100.0	30952	PASS
96	95	5	9	6.5	2014	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.5	25523	PASS
175	174	5	9	8.2	2092	PASS
176	174	95	105	95.4	24355	PASS
177	176	5	10	6.1	1474	PASS

m/z	Abundance
39.90	227.0
43.80	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
35.90	278.0
36.90	1736.0
37.90	1612.0
38.90	645.0
39.80	230.0
43.90	338.0
44.90	281.0
46.90	344.0
47.90	275.0
48.90	1448.0
50.00	6683.0
51.00	1987.0
52.00	109.0
54.90	190.0
55.90	583.0
56.90	1041.0
60.00	296.0
60.90	1683.0
61.90	1883.0
62.90	1226.0
63.80	190.0
67.00	140.0
67.90	3551.0
68.90	3654.0
69.90	292.0
71.90	247.0
72.90	1714.0
73.90	5986.0
75.00	17192.0
75.90	1428.0
77.00	163.0
77.80	158.0
78.90	1340.0
79.80	308.0
80.90	1370.0
81.80	299.0
86.80	1311.0
87.90	1201.0
90.80	172.0
91.90	884.0
93.00	1399.0
94.00	4052.0
95.00	30448.0
96.00	2029.0
103.80	205.0
105.70	161.0
115.80	101.0
116.80	254.0
117.80	141.0
118.80	174.0
127.90	106.0
129.70	103.0
140.90	423.0
142.80	414.0
172.00	115.0
173.90	24616.0
174.90	1988.0
175.90	23360.0
176.90	1500.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
35.90	299.0
36.90	1717.0
37.90	1688.0
38.90	670.0
39.80	241.0
43.90	345.0
44.90	285.0
46.90	349.0
47.90	261.0
48.90	1450.0
49.90	6815.0
51.00	2132.0
52.00	101.0
54.90	177.0
55.90	581.0
56.90	1014.0
60.00	352.0
60.90	1736.0
61.90	1918.0
62.90	1280.0
63.80	200.0
67.00	126.0
67.90	3596.0
68.90	3799.0
69.90	308.0
71.90	258.0
72.90	1717.0
73.90	6369.0
74.90	18200.0
75.90	1472.0
77.10	184.0
77.90	176.0
78.90	1406.0
79.80	354.0
80.80	1428.0
81.80	303.0
86.80	1372.0
87.90	1263.0
90.80	210.0
91.90	1000.0
92.90	1432.0
94.00	4204.0
95.00	31952.0
96.00	2072.0
103.80	211.0
105.80	150.0
116.80	265.0
117.80	166.0
118.80	189.0
127.90	120.0
129.70	106.0
140.80	383.0
142.80	484.0
172.00	143.0
173.90	26376.0
174.90	2138.0
175.90	25080.0
176.90	1496.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
35.90	316.0
37.00	1525.0
37.90	1515.0
38.90	574.0
39.80	269.0
43.90	369.0
44.90	268.0
46.90	371.0
47.90	217.0
48.90	1365.0
49.90	6297.0
51.00	2026.0
54.80	157.0
55.80	531.0
56.90	950.0
59.90	397.0
60.90	1683.0
61.90	1702.0
62.90	1185.0
63.80	216.0
66.90	105.0
67.90	3331.0
68.90	3609.0
69.90	278.0
71.90	219.0
72.90	1587.0
73.90	6196.0
74.90	17296.0
76.00	1436.0
76.80	192.0
77.00	190.0
77.90	165.0
78.90	1325.0
79.80	392.0
80.80	1279.0
81.80	261.0
86.80	1241.0
87.90	1237.0
90.80	214.0
91.90	1018.0
92.90	1320.0
94.00	3977.0
95.00	30456.0
96.00	1941.0
103.80	173.0
105.80	142.0
115.60	102.0
116.80	263.0
117.80	188.0
118.90	204.0
127.90	125.0
129.70	106.0
140.80	328.0
142.80	464.0
172.10	147.0
173.90	25576.0
174.90	2150.0
175.90	24624.0
176.90	1425.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256