




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012325\
 Data File : VV038513.D
 Acq On : 23 Jan 2025 18:00
 Operator : SY/MD
 Sample : Q1137-04DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAB3DL

Manual IntegrationsAPPROVED

Quant Time: Jan 24 01:41:34 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 24 00:30:49 2025
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/03/2025
 Supervised By :Semsettin Yesilyurt 02/03/2025

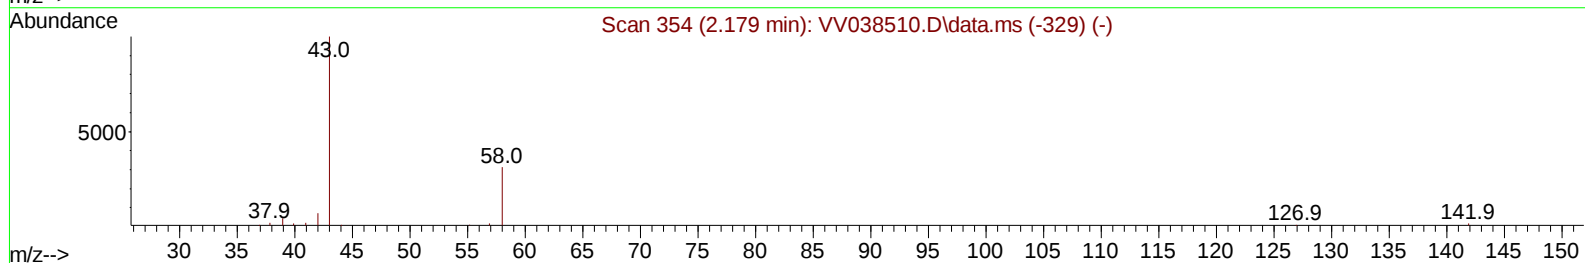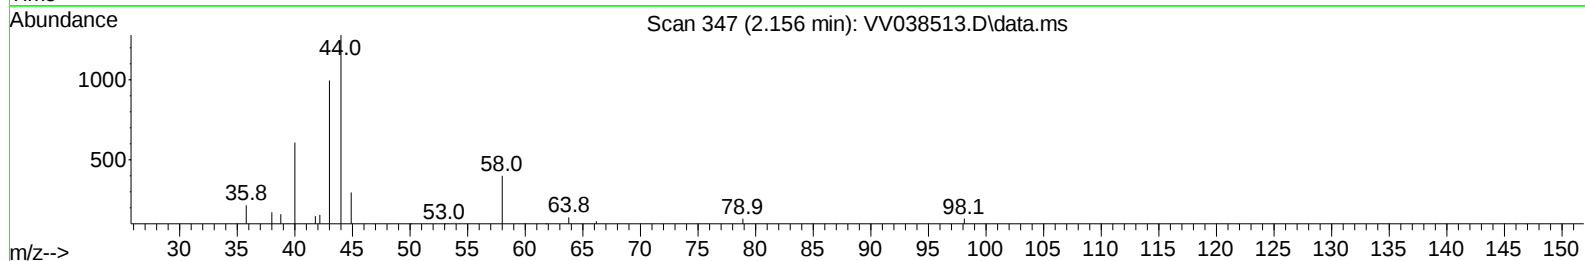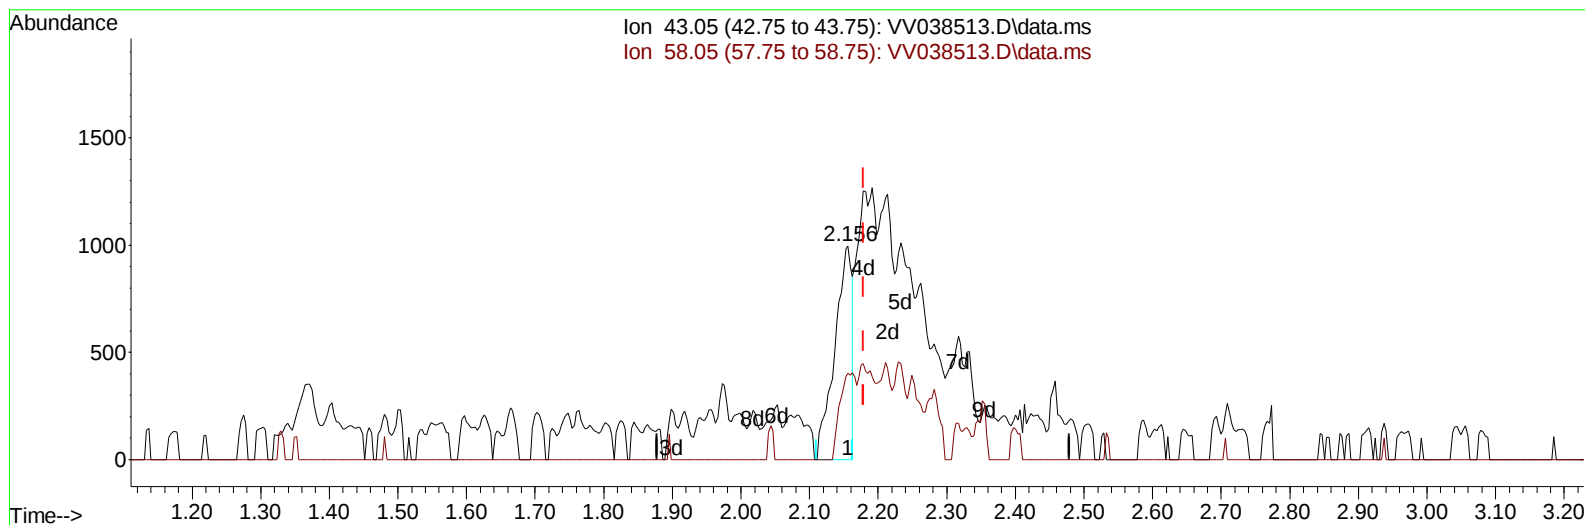

TIC: VV038513.D\data.ms

(13) Acetone (T)

2.156min (-0.023) 0.67 ug/L

response 1738

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.60	38.38
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012325\
 Data File : VV038513.D
 Acq On : 23 Jan 2025 18:00
 Operator : SY/MD
 Sample : Q1137-04DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAB3DL

Manual IntegrationsAPPROVED

Quant Time: Jan 24 00:32:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725wMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 24 00:30:49 2025
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/03/2025
 Supervised By :Semsettin Yesilyurt 02/03/2025

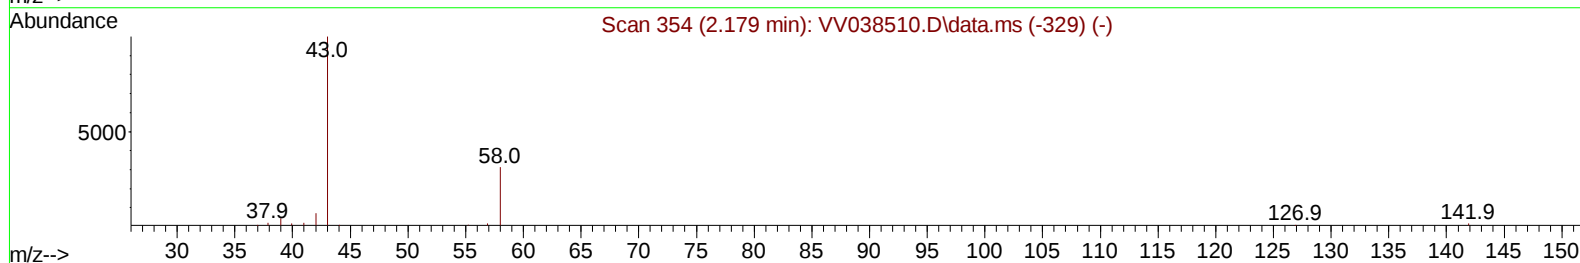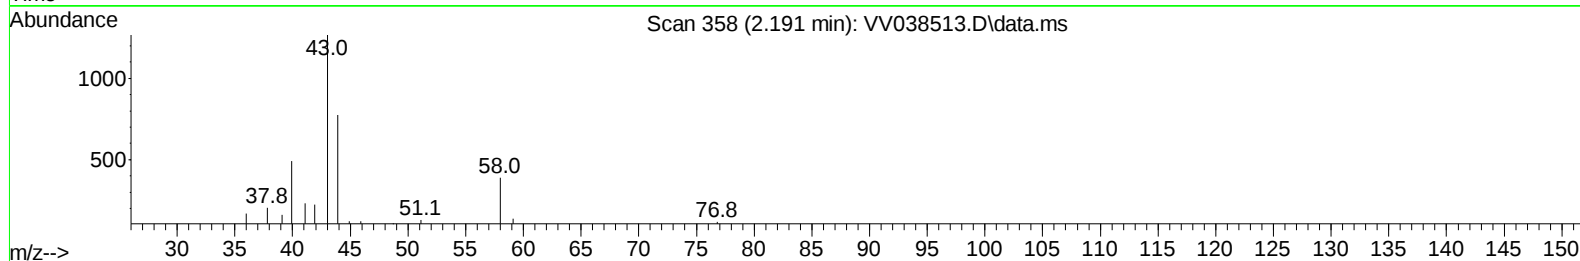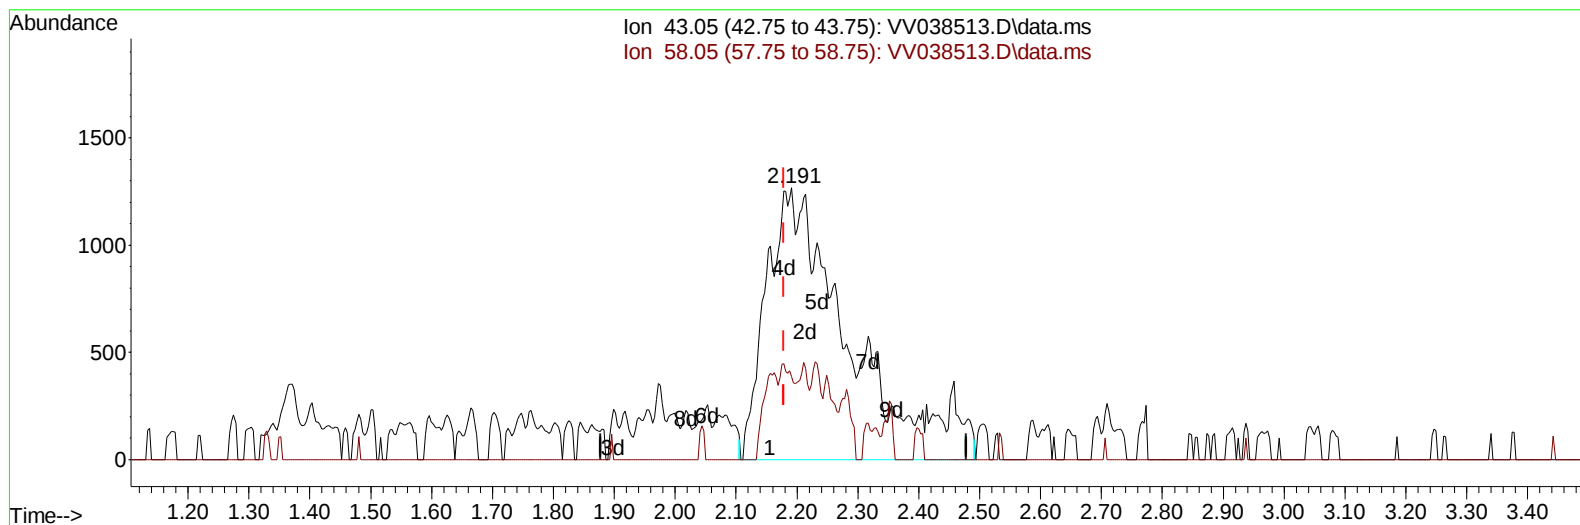

TIC: VV038513.D\data.ms

(13) Acetone (T)

2.191min (+ 0.013) 4.61 ug/L m

response 11891

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.60	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012325\
 Data File : VV038513.D
 Acq On : 23 Jan 2025 18:00
 Operator : SY/MD
 Sample : Q1137-04DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAB3DL

Manual IntegrationsAPPROVED

Quant Time: Jan 24 00:32:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 24 00:30:49 2025
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/03/2025
 Supervised By :Semsettin Yesilyurt 02/03/2025

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.529	114		190945	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117		204292	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152		86785	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		51852	3.293	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	65.800%		
7) Chloroethane-d5	1.532	69		51927	3.927	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	78.600%		
11) 1,1-Dichloroethene-d2	2.056	65		26129	3.682	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	73.600%		
20) 2-Butanone-d5	3.850	46		119952	36.219	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130		Recovery =	72.440%		
24) Chloroform-d	4.243	84		126163	4.275	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	85.400%		
26) 1,2-Dichloroethane-d4	4.940	65		57843	4.277	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	85.600%		
32) Benzene-d6	4.953	84		223353	3.970	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	79.400%		
36) 1,2-Dichloropropane-d6	5.982	67		74186	4.338	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	86.800%		
41) Toluene-d8	7.236	98		175087	3.464	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	69.200%#		
43) trans-1,3-Dichloroprop...	7.558	79		23075	3.688	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	73.800%		
46) 2-Hexanone-d5	8.027	63		88224	35.745	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	71.480%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84		60751	4.481	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	89.600%		
66) 1,2-Dichlorobenzene-d4	11.554	152		67272	4.580	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	91.600%		
Target Compounds							
3) Chloromethane	1.214	50		165258	7.551	ug/L	99
13) Acetone	2.191	43		11891m	4.615	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012325\
Data File : VV038513.D
Acq On : 23 Jan 2025 18:00
Operator : SY/MD
Sample : Q1137-04DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAB3DL

Manual IntegrationsAPPROVED

Quant Time: Jan 24 00:32:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 24 00:30:49 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 02/03/2025
Supervised By :Semsettin Yesilyurt 02/03/2025

