
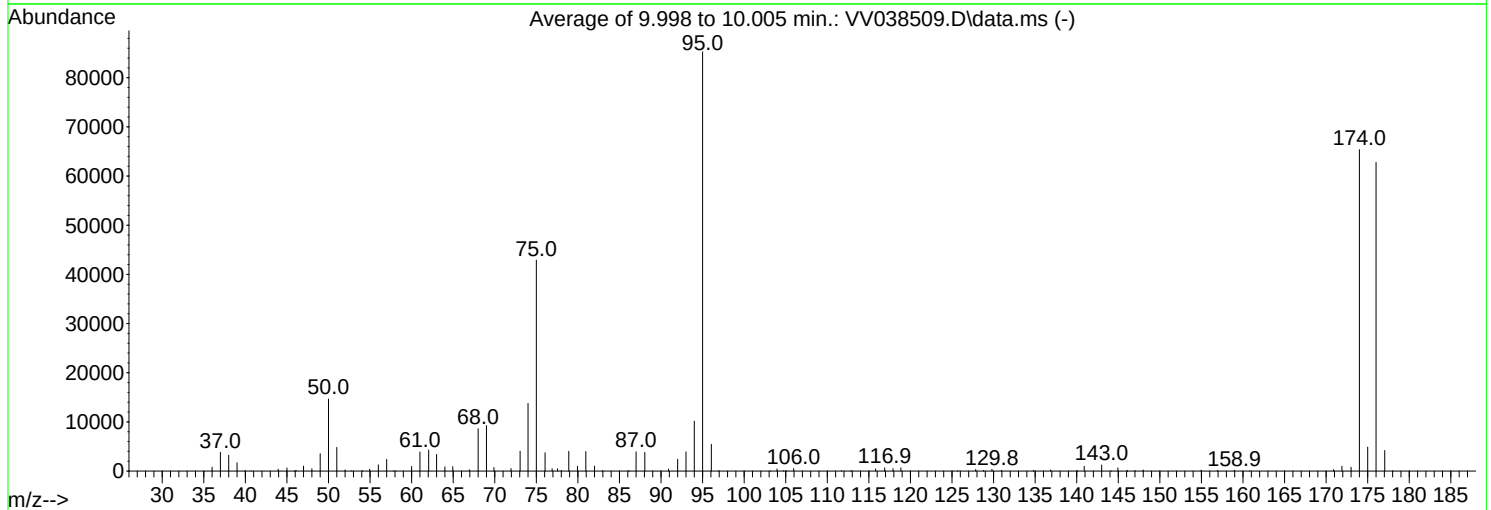


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012325\
Data File : VV038509.D
Acq On : 23 Jan 2025 15:25
Operator : SY/MD
Sample : BFB401
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB401

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jan 24 00:30:49 2025

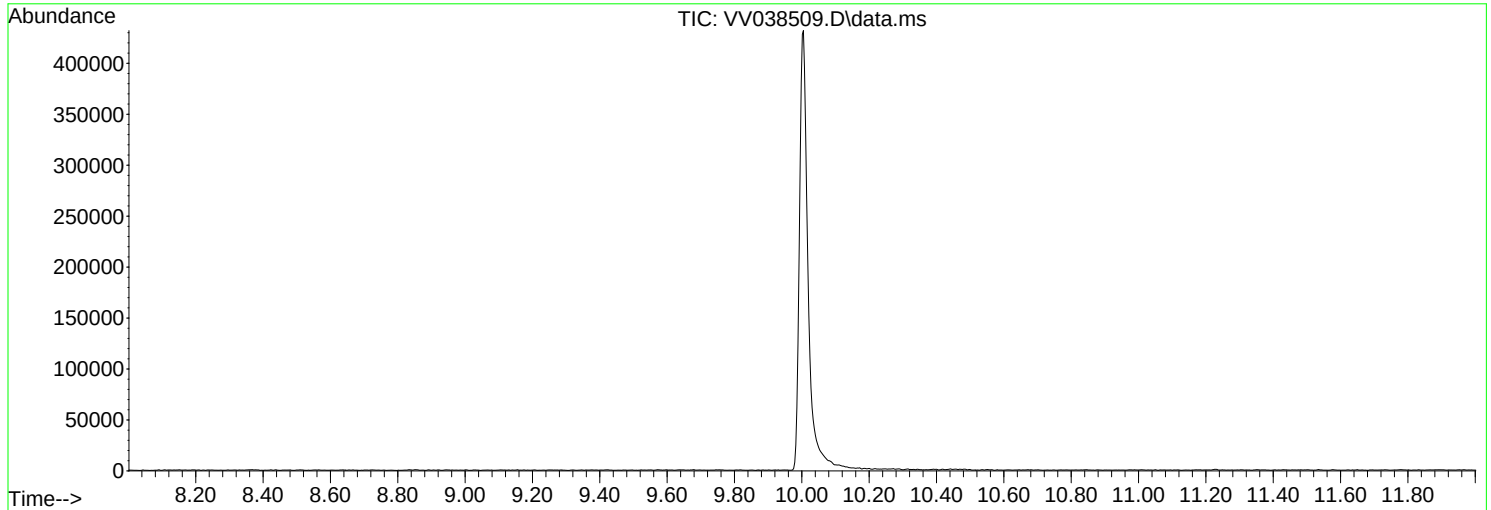

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	14659	PASS
75	95	30	80	50.3	42907	PASS
95	95	100	100	100.0	85280	PASS
96	95	5	9	6.4	5462	PASS
173	174	0.00	2	1.2	792	PASS
174	95	50	120	76.7	65379	PASS
175	174	5	9	7.5	4876	PASS
176	174	95	105	96.0	62787	PASS
177	176	5	10	6.7	4190	PASS

m/z	Abundance
40.00	325.0
43.90	370.0

Instrument :
MSVOA_V
ClientSampleId :
BFB401

m/z	Abundance
36.00	771.0
37.00	3383.0
38.00	3146.0
39.00	1566.0
39.90	392.0
44.00	690.0
45.00	541.0
45.90	177.0
47.00	819.0
48.00	473.0
49.00	3207.0
50.00	13853.0
51.00	4547.0
52.10	279.0
55.00	276.0
56.00	1227.0
57.00	2276.0
57.80	120.0
60.00	931.0
61.00	3684.0
62.00	4127.0
63.00	3156.0
64.00	745.0
64.90	855.0
66.90	276.0
68.00	7990.0
69.00	8439.0
69.90	764.0
71.90	482.0
73.00	3708.0
74.00	12882.0
75.00	39960.0
76.10	3298.0
76.90	389.0
77.50	529.0
78.90	3736.0
79.90	808.0
81.00	3687.0
82.00	952.0
86.20	140.0
87.00	3586.0
88.00	3465.0
90.90	433.0
92.00	2272.0
93.00	3333.0
94.00	9726.0
95.00	80384.0
96.00	5431.0
96.90	165.0
104.00	402.0
106.00	457.0
112.90	143.0
115.80	411.0
116.90	561.0
117.90	438.0
118.80	594.0
127.90	358.0
128.80	116.0
129.80	375.0
131.00	112.0
134.80	107.0
136.90	171.0
140.00	103.0
140.90	886.0
143.00	1141.0
145.00	618.0
146.10	110.0
147.00	120.0
148.10	221.0
154.90	138.0
157.00	124.0
159.00	164.0
160.80	101.0
170.90	326.0
171.80	778.0
173.00	686.0
174.00	58448.0
175.00	4511.0
176.00	56368.0
177.00	4000.0

Instrument :
MSVOA_V
ClientSampleId :
BFB401

m/z	Abundance
36.00	833.0
37.00	3963.0
38.00	3330.0
39.00	1752.0
39.90	390.0
40.70	108.0
44.00	796.0
45.00	661.0
46.10	197.0
47.00	1046.0
48.00	465.0
49.00	3652.0
50.00	15171.0
51.00	4880.0
52.00	249.0
52.80	106.0
54.10	122.0
54.90	387.0
56.00	1322.0
57.00	2443.0
60.00	985.0
61.00	3980.0
62.00	4410.0
63.00	3428.0
64.00	893.0
65.00	969.0
67.00	271.0
68.00	8917.0
69.00	9624.0
69.90	770.0
71.90	537.0
73.10	4202.0
74.00	14282.0
75.00	44240.0
76.10	3901.0
76.90	489.0
77.50	535.0
78.90	4227.0
80.00	982.0
80.90	4174.0
82.00	1081.0
82.90	126.0
86.20	124.0
87.00	4049.0
88.10	3976.0
90.90	410.0
92.00	2517.0
93.00	4122.0
94.00	10433.0
95.00	88312.0
96.10	5596.0
97.00	120.0
103.20	101.0
104.00	448.0
104.70	133.0
105.10	137.0
106.00	555.0
111.70	103.0
112.90	131.0
115.80	467.0
116.90	678.0
117.90	543.0
118.80	686.0
125.70	113.0
127.90	342.0
128.80	143.0
129.80	405.0
130.90	169.0
134.80	146.0
136.90	239.0
140.10	124.0
140.90	1017.0
143.00	1269.0
144.20	102.0
144.90	691.0
146.10	170.0
147.00	113.0
148.00	242.0
155.00	187.0
156.90	148.0
158.90	192.0
170.90	293.0
171.90	986.0
173.00	794.0
174.00	67520.0
175.00	5065.0
176.00	65080.0
177.00	4317.0

Instrument :
MSVOA_V
ClientSampleId :
BFB401

m/z	Abundance
36.00	807.0
37.00	4087.0
38.00	3203.0
39.00	1763.0
40.00	329.0
44.00	802.0
45.00	734.0
46.10	257.0
47.00	1181.0
48.00	497.0
49.00	3757.0
50.00	14954.0
51.00	5013.0
51.90	220.0
52.80	106.0
54.10	120.0
54.90	468.0
56.00	1270.0
57.00	2395.0
58.10	135.0
60.00	905.0
61.00	4001.0
62.10	4335.0
63.00	3546.0
64.00	941.0
65.00	921.0
67.00	264.0
68.00	8984.0
69.00	9679.0
69.90	640.0
72.00	535.0
73.10	4213.0
74.00	14158.0
75.00	44520.0
76.00	3994.0
76.90	607.0
77.60	363.0
78.00	347.0
78.90	4098.0
80.00	1144.0
80.90	4096.0
82.00	1037.0
83.00	142.0
86.10	157.0
87.00	4130.0
88.00	3945.0
90.90	387.0
92.00	2451.0
93.00	4300.0
94.00	10291.0
95.00	87144.0
96.10	5358.0
103.90	472.0
104.80	166.0
105.90	537.0
111.70	136.0
112.70	138.0
115.80	452.0
116.90	765.0
117.90	508.0
118.90	694.0
125.70	117.0
127.80	288.0
128.80	166.0
129.80	358.0
131.00	185.0
134.80	180.0
136.80	245.0
140.10	102.0
140.90	994.0
143.00	1308.0
144.90	615.0
146.10	171.0
147.00	100.0
147.90	197.0
155.00	203.0
156.90	182.0
158.90	190.0
170.90	286.0
172.00	1191.0
173.00	895.0
174.00	70168.0
175.00	5051.0
176.00	66912.0
177.10	4254.0
178.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB401