


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV012419\
 Data File : VV009252.D
 Acq On : 24 Jan 2019 09:32
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\82V012419S.M
 Title : SW846 8260
 Last Update : Thu Jan 24 23:18:07 2019

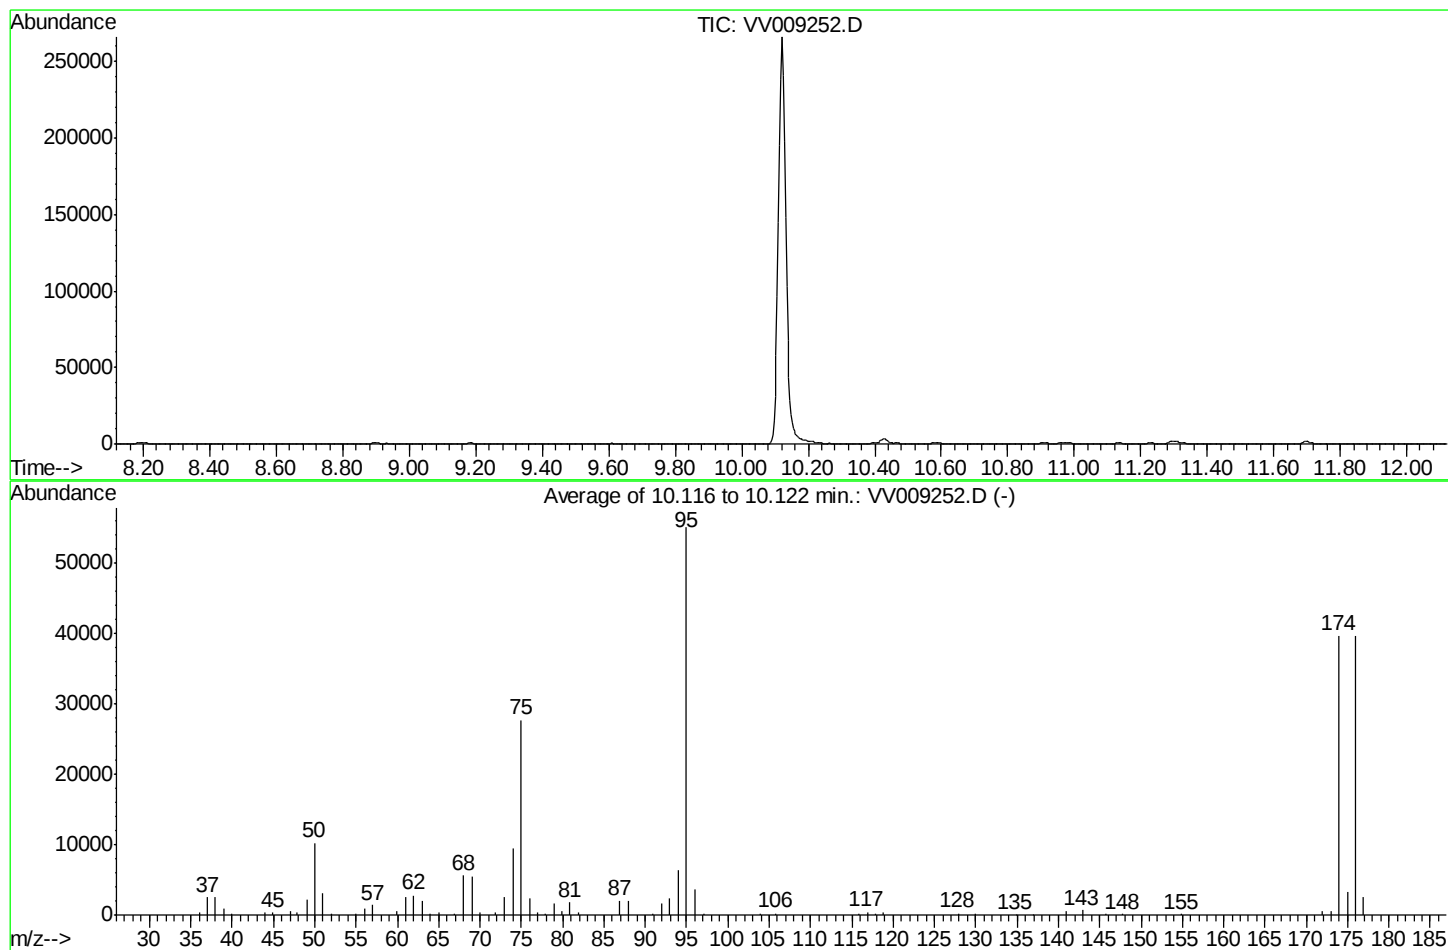

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	10211	PASS
75	95	30	60	50.3	27696	PASS
95	95	100	100	100.0	55024	PASS
96	95	5	9	6.6	3633	PASS
173	174	0.00	2	1.5	600	PASS
174	95	50	100	72.1	39664	PASS
175	174	5	9	8.1	3200	PASS
176	174	95	101	99.8	39581	PASS
177	176	5	9	6.4	2515	PASS