
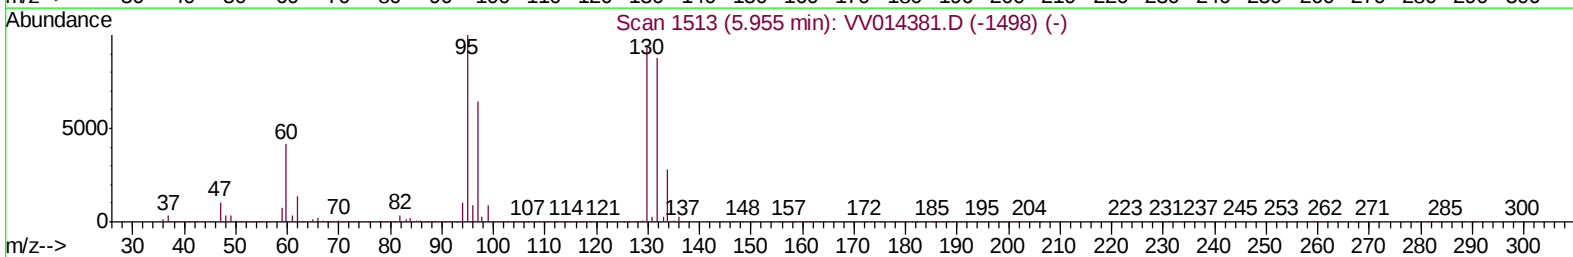
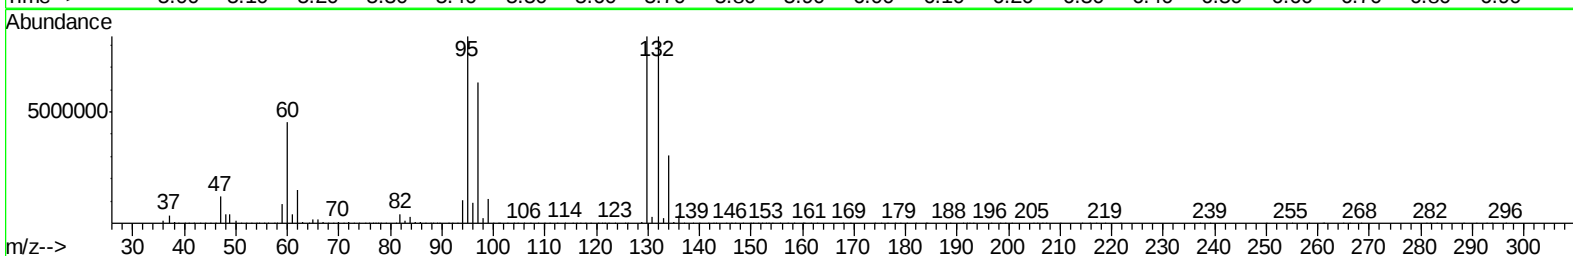


Data File : VV014396.D
Acq On : 24 Jan 2020 18:22
Operator : SY/MD
Sample : L1253-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jan 25 00:24:19 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 25 00:18:39 2020
Response via : Initial Calibration

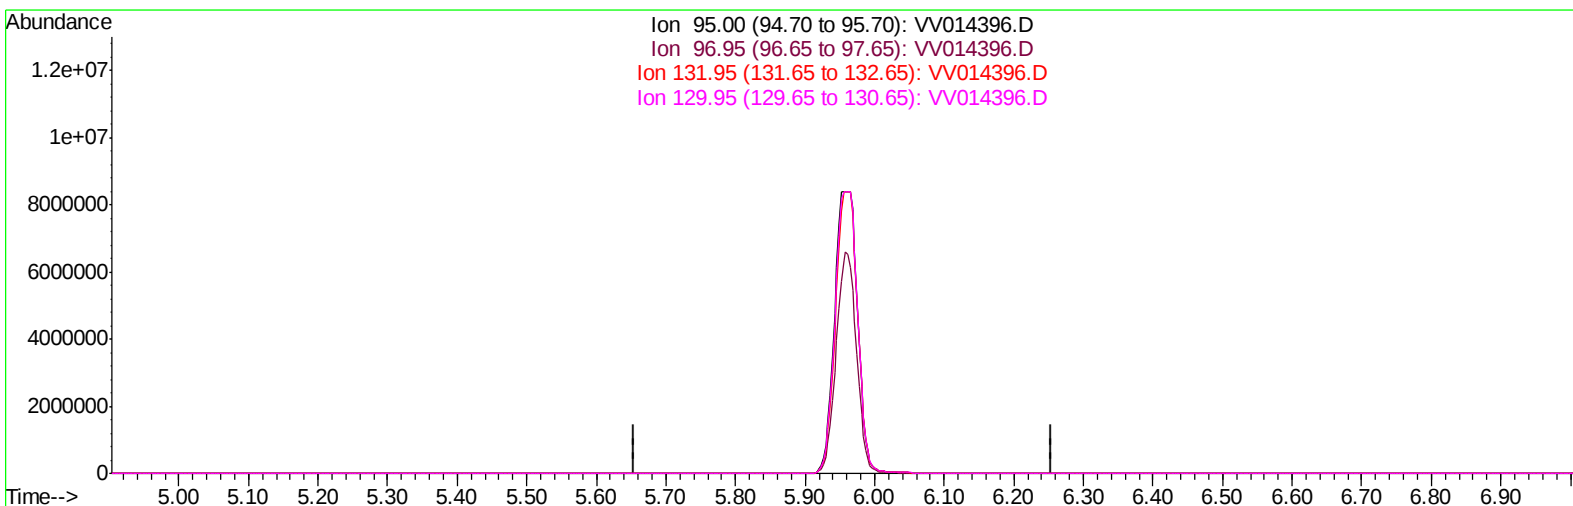

TIC: VV014396.D

(34) Trichloroethene (T)

5.955min (-5.955) 0.00ug/L

response 0

Ion	Exp%	Act%
95.00	100	0.00
96.95	62.50	0.00#
131.95	90.60	0.00#
129.95	93.90	0.00#