

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV012420\
 Data File : VV014396.D
 Acq On : 24 Jan 2020 18:22
 Operator : SY/MD
 Sample : L1253-05
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AC2

Manual Integrations
 APPROVED

MMDadoda
 1/27/2020 2:57:03 PM

Quant Time: Jan 27 09:07:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 25 00:18:39 2020
 Response via : Initial Calibration

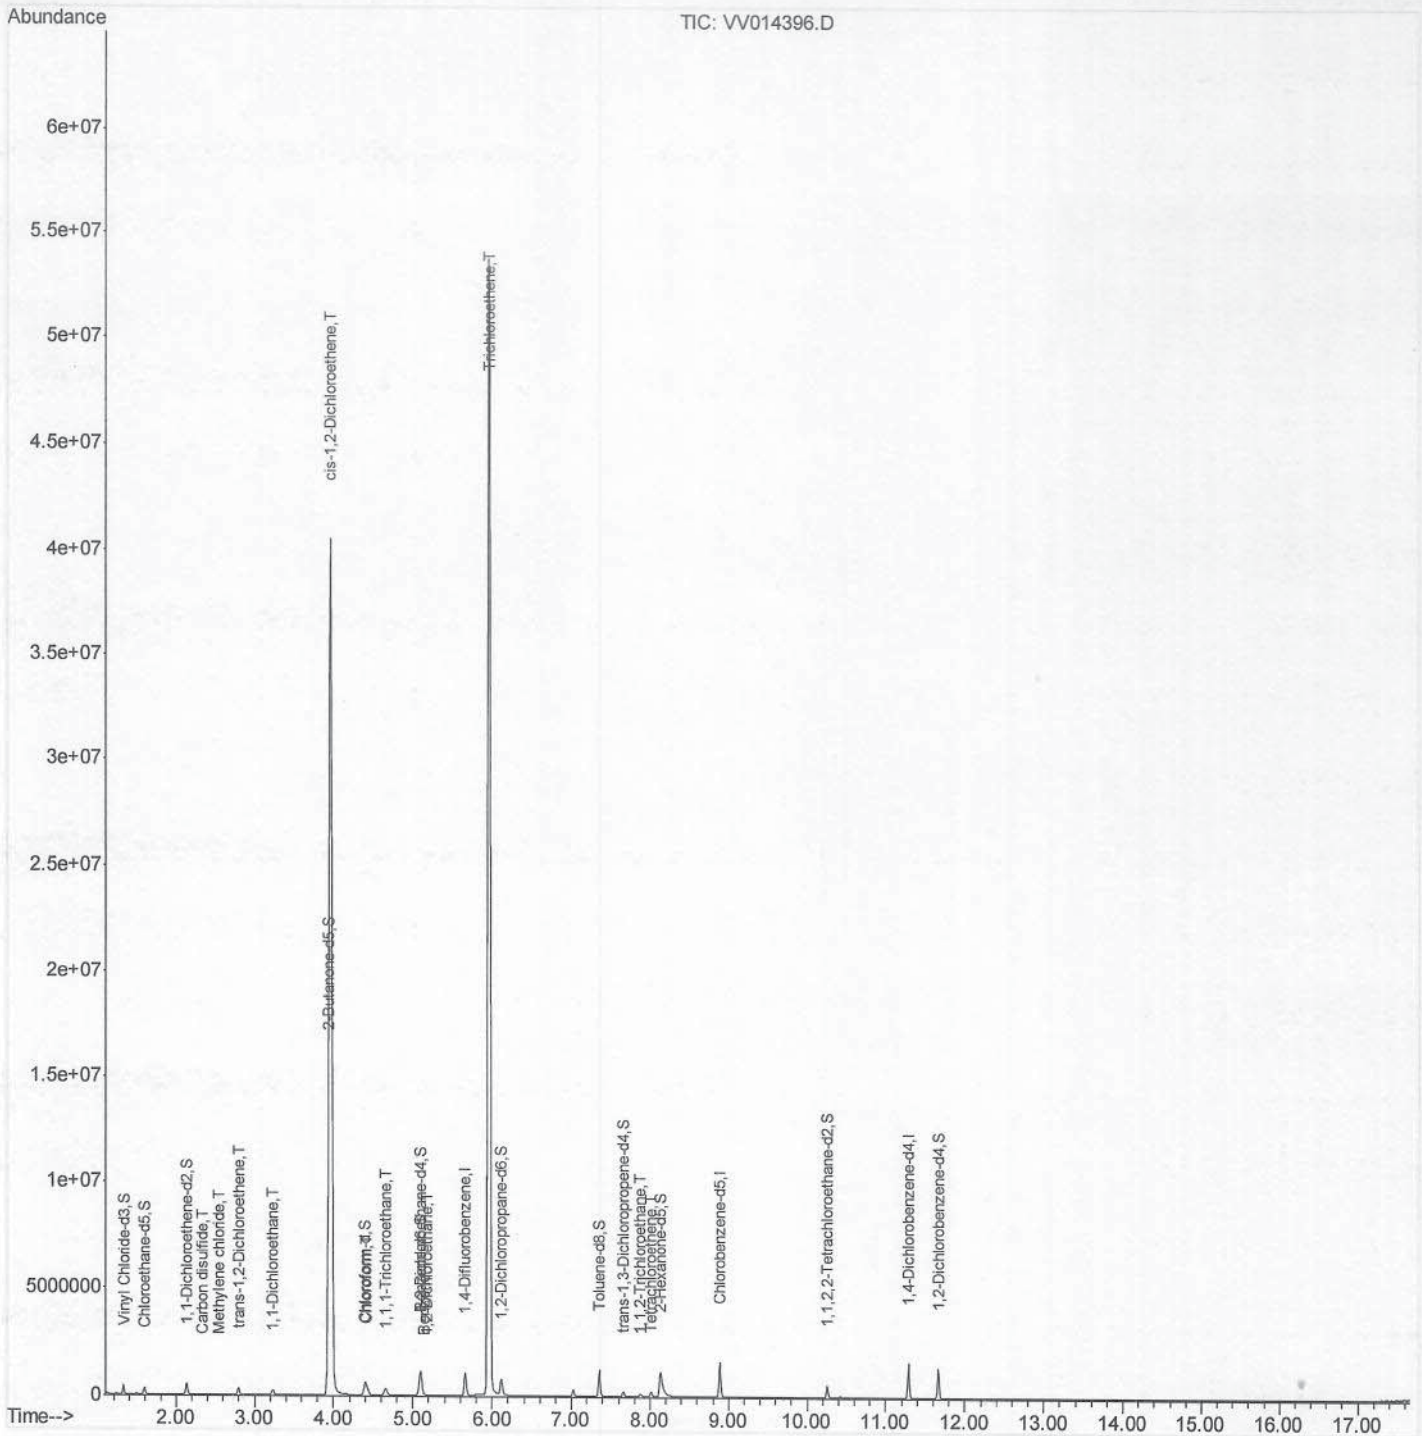

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV012420\
Quantitation Report (Qedit)




Data File : VV014396.D
Acq On : 24 Jan 2020 18:22
Operator : SY/MD
Sample : L1253-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC2

Manual Integrations
APPROVED

MMDadoda
1/27/2020 2:57:03 PM

Quant Time: Jan 25 00:24:19 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 25 00:18:39 2020
Response via : Initial Calibration

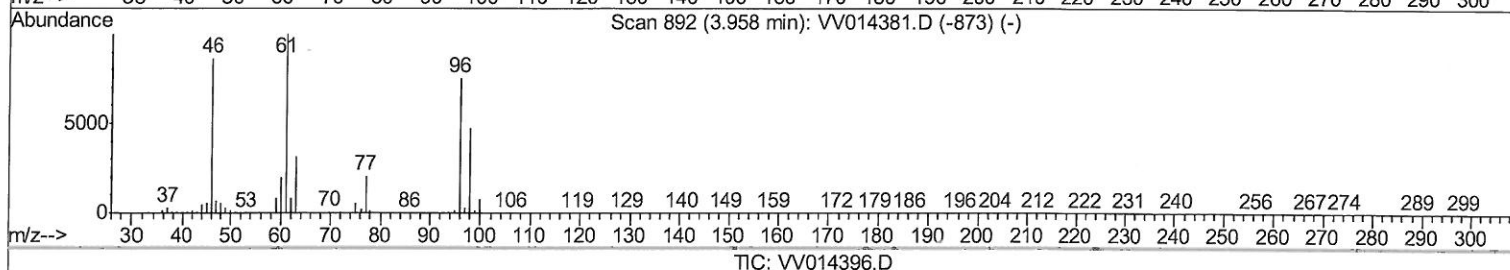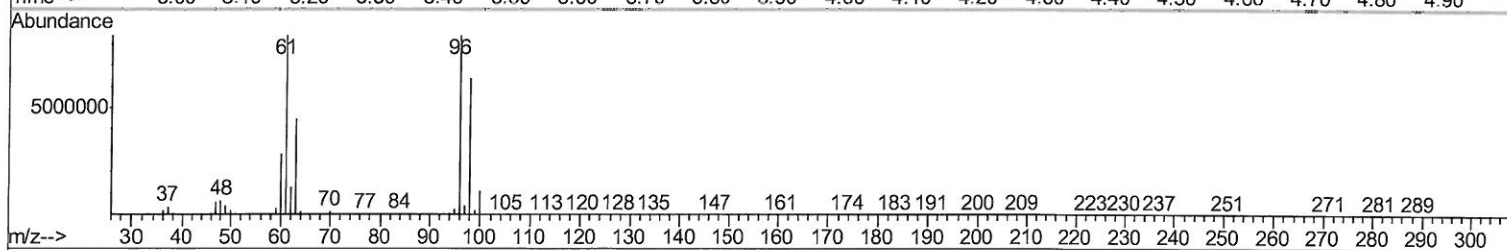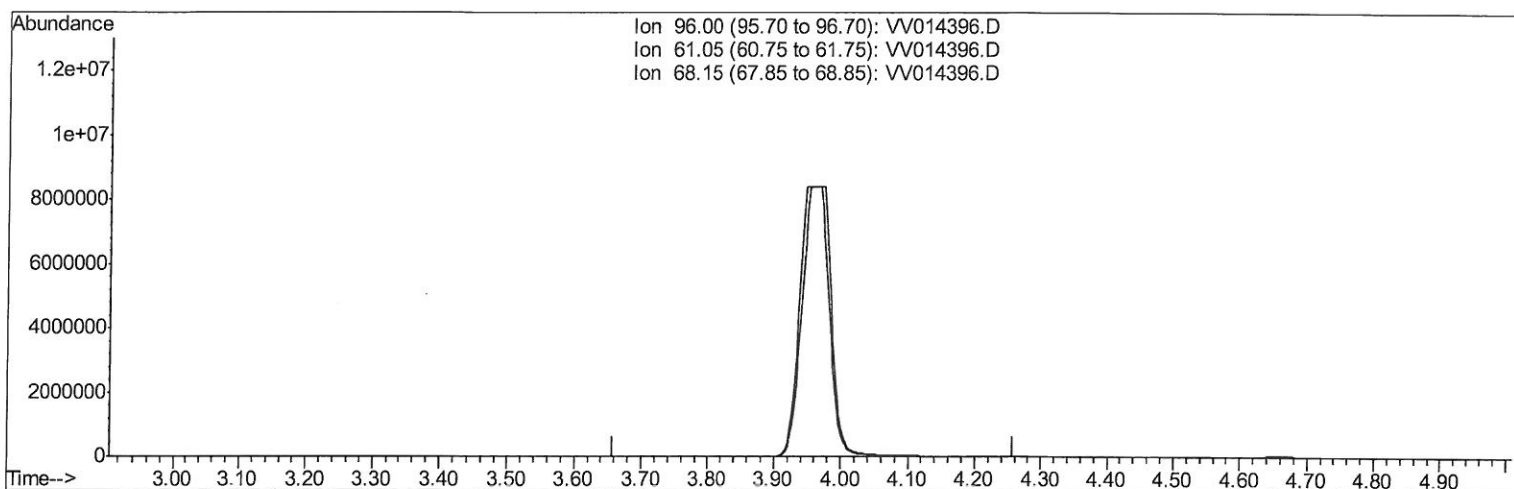

(22) cis-1,2-Dichloroethene (T)

3.958min (-3.958) 0.00ug/L

response 0

Ion	Exp%	Act%
96.00	100	0.00
61.05	129.50	0.00#
68.15	0.50	0.00#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV012420\
Quantitation Report (Qedit)




Data File : VV014396.D
Acq On : 24 Jan 2020 18:22
Operator : SY/MD
Sample : L1253-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC2

Manual Integrations
APPROVED

MMDadoda
1/27/2020 2:57:03 PM

Quant Time: Jan 25 00:24:19 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 25 00:18:39 2020
Response via : Initial Calibration

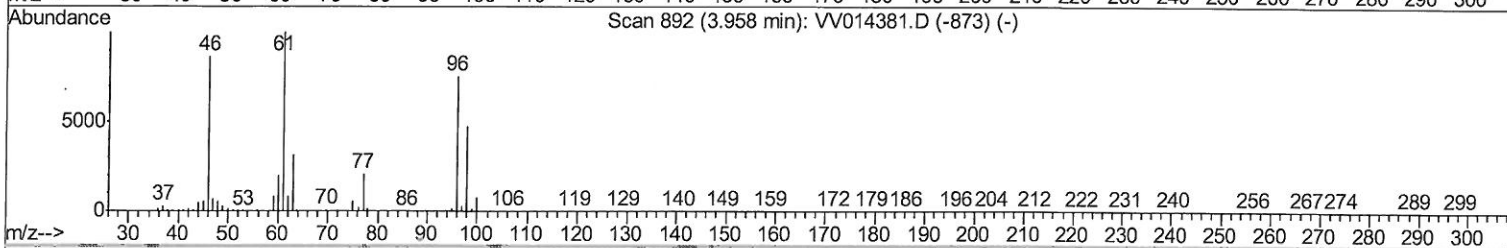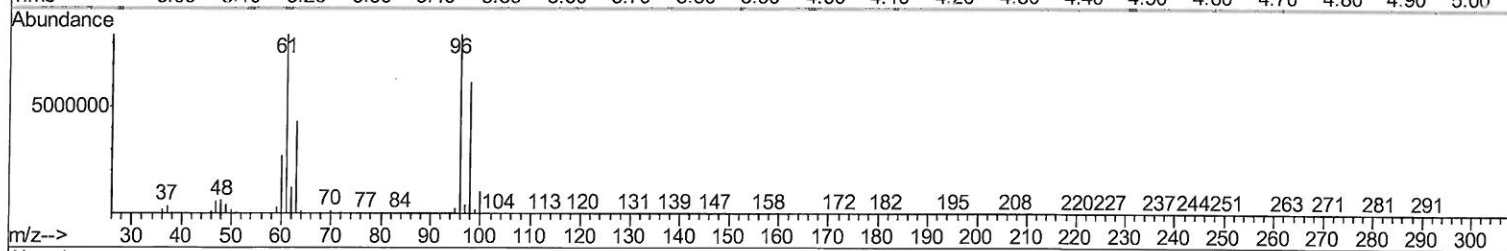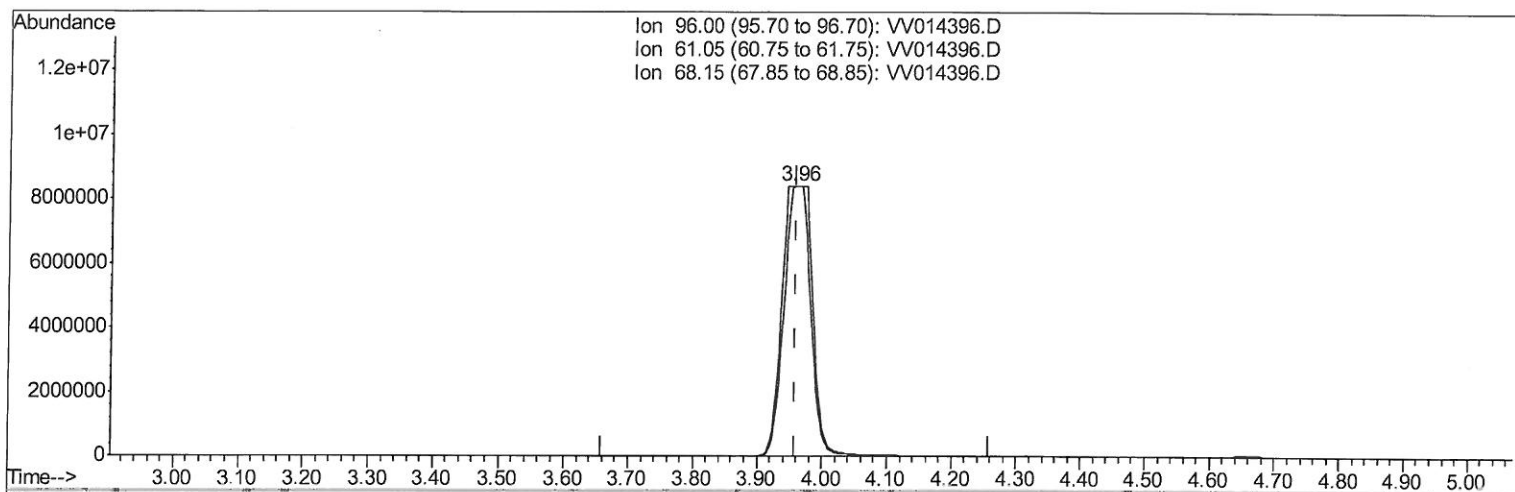

TIC: VV014396.D

(22) cis-1,2-Dichloroethene (T)

3.955min (-0.003) 343.70ug/L m

response 23589311

Ion	Exp%	Act%
96.00	100	100
61.05	129.50	100.00
68.15	0.50	0.00#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV012420\
Quantitation Report (Qedit)




Data File : VV014396.D
Acq On : 24 Jan 2020 18:22
Operator : SY/MD
Sample : L1253-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC2

Manual Integrations
APPROVED

MMDadoda
1/27/2020 2:57:03 PM

Quant Time: Jan 25 00:24:19 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 25 00:18:39 2020
Response via : Initial Calibration

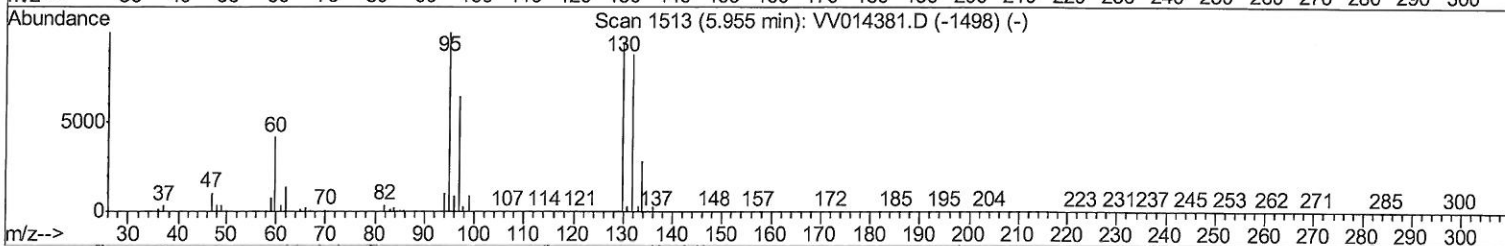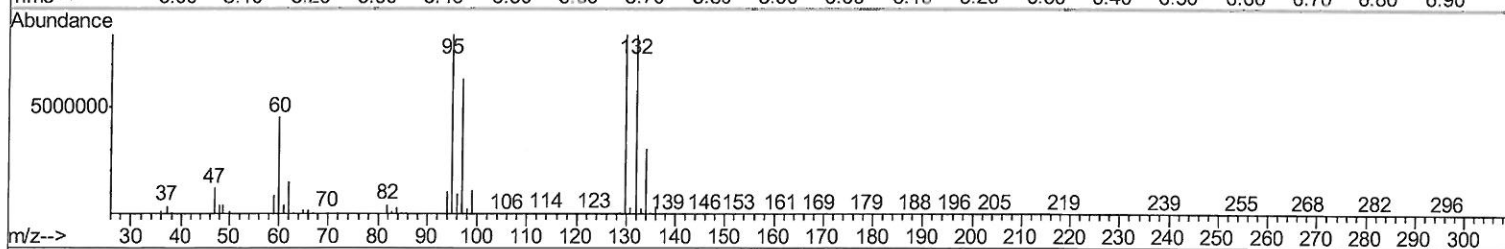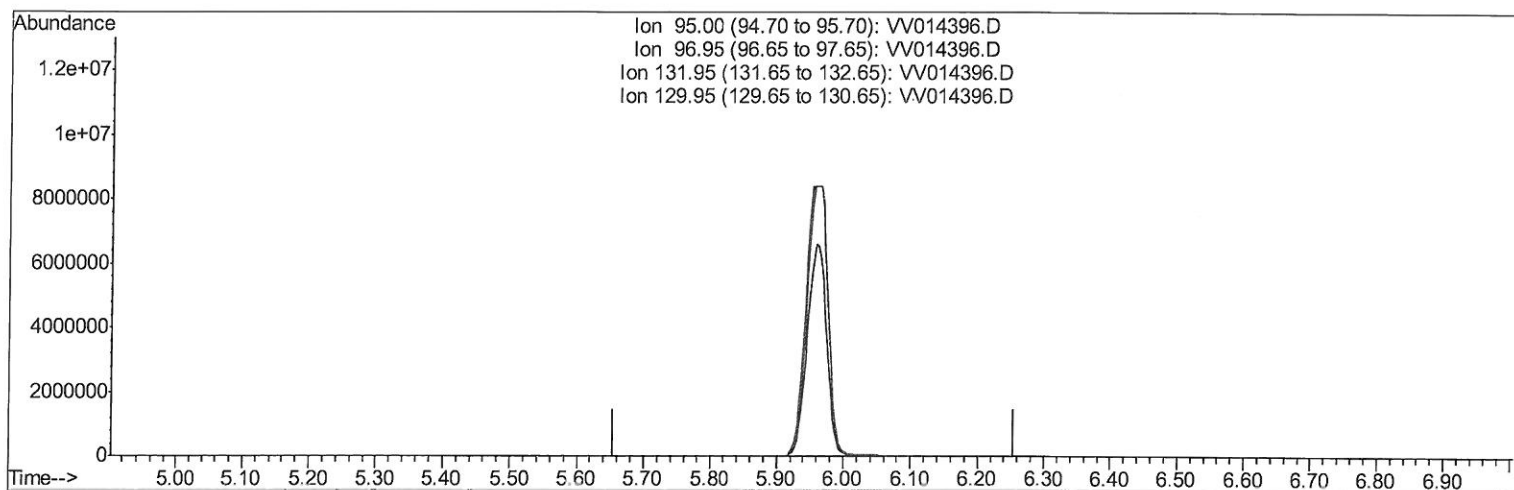

TIC: VV014396.D

(34) Trichloroethene (T)

5.955min (-5.955) 0.00ug/L

response 0

Ion	Exp%	Act%
95.00	100	0.00
96.95	62.50	0.00#
131.95	90.60	0.00#
129.95	93.90	0.00#

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV012420\
Quantitation Report (Qedit)




Data File : VV014396.D
Acq On : 24 Jan 2020 18:22
Operator : SY/MD
Sample : L1253-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC2

Manual Integrations
APPROVED

MMDadoda
1/27/2020 2:57:03 PM

Quant Time: Jan 25 00:24:19 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 25 00:18:39 2020
Response via : Initial Calibration

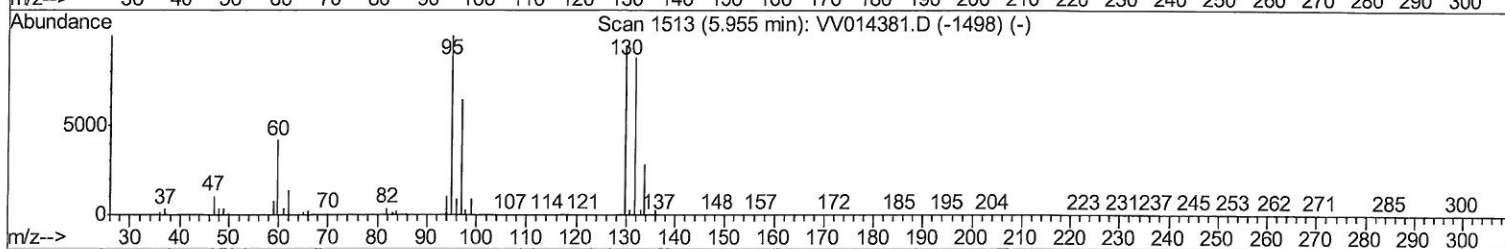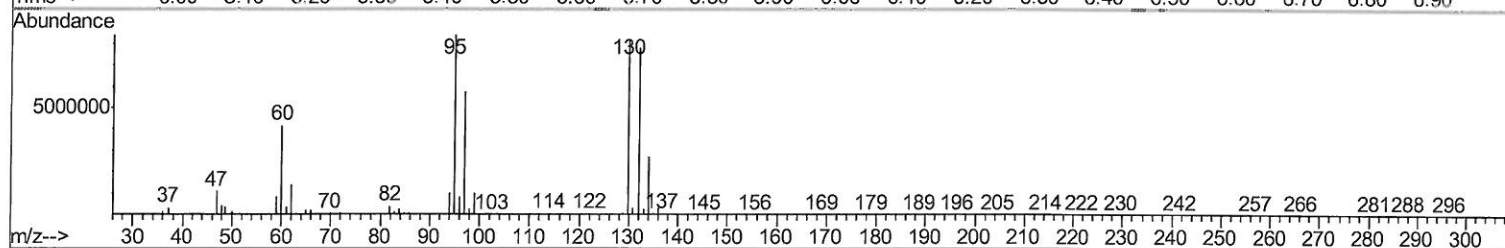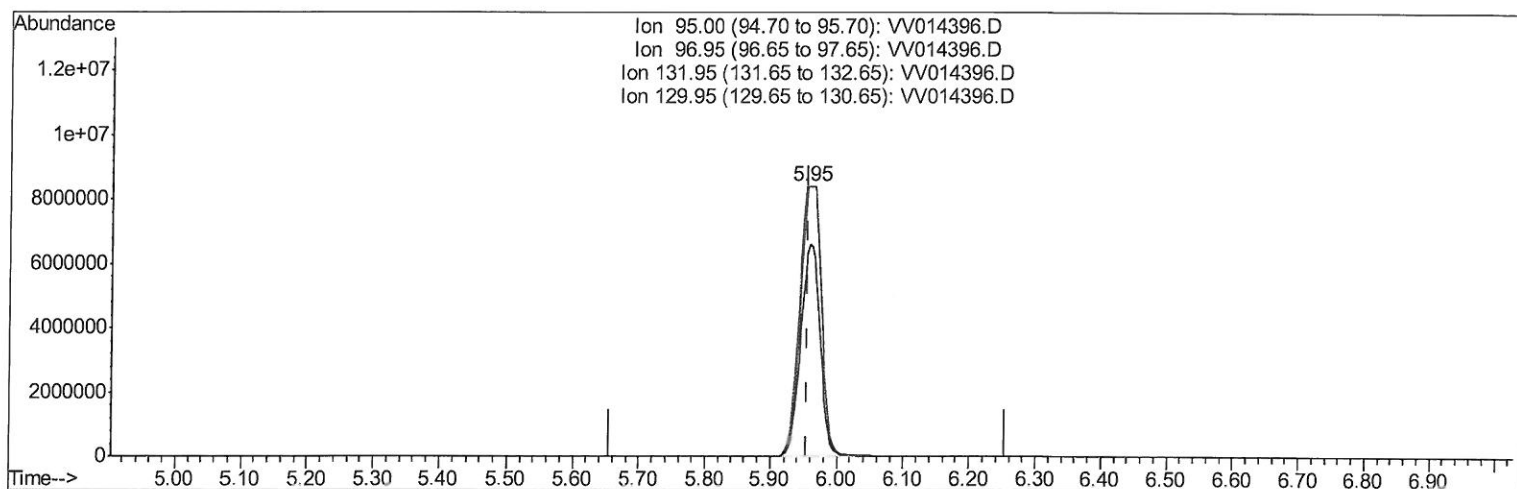

TIC: VV014396.D

(34) Trichloroethene (T)

5.952min (-0.003) 284.42ug/L m

response 19268886

Ion	Exp%	Act%
95.00	100	100
96.95	62.50	68.40
131.95	90.60	93.02
129.95	93.90	97.14

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV012420\
 Data File : VV014396.D
 Acq On : 24 Jan 2020 18:22
 Operator : SY/MD
 Sample : L1253-05
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AC2

Manual Integrations
 APPROVED

MMDadoda
 1/27/2020 2:57:03 PM

Quant Time: Jan 27 09:07:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 25 00:18:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	932283	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	856024	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	394958	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	240891	3.69	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.80%
7) Chloroethane-d5	1.59	69	218860	4.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.80%
11) 1,1-Dichloroethene-d2	2.14	63	262156	2.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.60%#
20) 2-Butanone-d5	3.93	46	834473	53.25	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.50%
24) Chloroform-d	4.40	84	569270	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.20%
26) 1,2-Dichloroethane-d4	5.08	65	285181	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.20%
32) Benzene-d6	5.10	84	1050833	4.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.20%
36) 1,2-Dichloropropane-d6	6.12	67	367607	4.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.80%
41) Toluene-d8	7.36	98	827980	3.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.00%
43) trans-1,3-Dichloropropene-	7.66	79	129133	3.69	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.80%
46) 2-Hexanone-d5	8.13	63	766807	51.69	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.38%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	293252	5.29	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	334671	4.51	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.20%

Target Compounds

					Ovalue	
14) Carbon disulfide	2.32	76	24913	0.135	ug/L	96
16) Methylene chloride	2.54	84	11867	0.175	ug/L	90
18) trans-1,2-Dichloroethene	2.79	96	130042	2.077	ug/L	94
19) 1,1-Dichloroethane	3.23	63	234227	1.909	ug/L	95
22) cis-1,2-Dichloroethene	3.96	96	23589311m	343.704	ug/L	95
25) Chloroform	4.42	83	244972	2.085	ug/L	98
27) 1,2-Dichloroethane	5.18	62	11740	0.167	ug/L #	69
29) 1,1,1-Trichloroethane	4.66	97	262171	2.573	ug/L	100
33) Benzene	5.15	78	19243	0.073	ug/L	100
34) Trichloroethene	5.95	95	19268886m	284.423	ug/L	97
45) 1,1,2-Trichloroethane	7.88	97	46967	1.105	ug/L	97
47) Tetrachloroethene	8.02	164	46444	1.003	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed