

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV012420\
 Data File : VV014382.D
 Acq On : 24 Jan 2020 11:46
 Operator : SY/MD
 Sample : VV0124WBL01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK55

Quant Time: Jan 25 00:37:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 25 00:18:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	940367	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	863841	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	387223	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	258676	3.93	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.60%
7) Chloroethane-d5	1.58	69	216119	4.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.00%
11) 1,1-Dichloroethene-d2	2.13	63	334847	3.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.00%
20) 2-Butanone-d5	3.95	46	598859	37.89	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	75.78%
24) Chloroform-d	4.40	84	608735	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
26) 1,2-Dichloroethane-d4	5.08	65	293663	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.20%
32) Benzene-d6	5.09	84	1302215	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
36) 1,2-Dichloropropane-d6	6.11	67	406789	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	7.35	98	1203717	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.20%
43) trans-1,3-Dichloropropene-	7.66	79	157068	4.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.80%
46) 2-Hexanone-d5	8.13	63	696336	46.52	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.04%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	268231	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	376620	5.18	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.60%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	24870	0.364 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV012420\
Data File : VV014382.D
Acq On : 24 Jan 2020 11:46
Operator : SY/MD
Sample : VV0124WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK55

Quant Time: Jan 25 00:37:05 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 25 00:18:39 2020
Response via : Initial Calibration

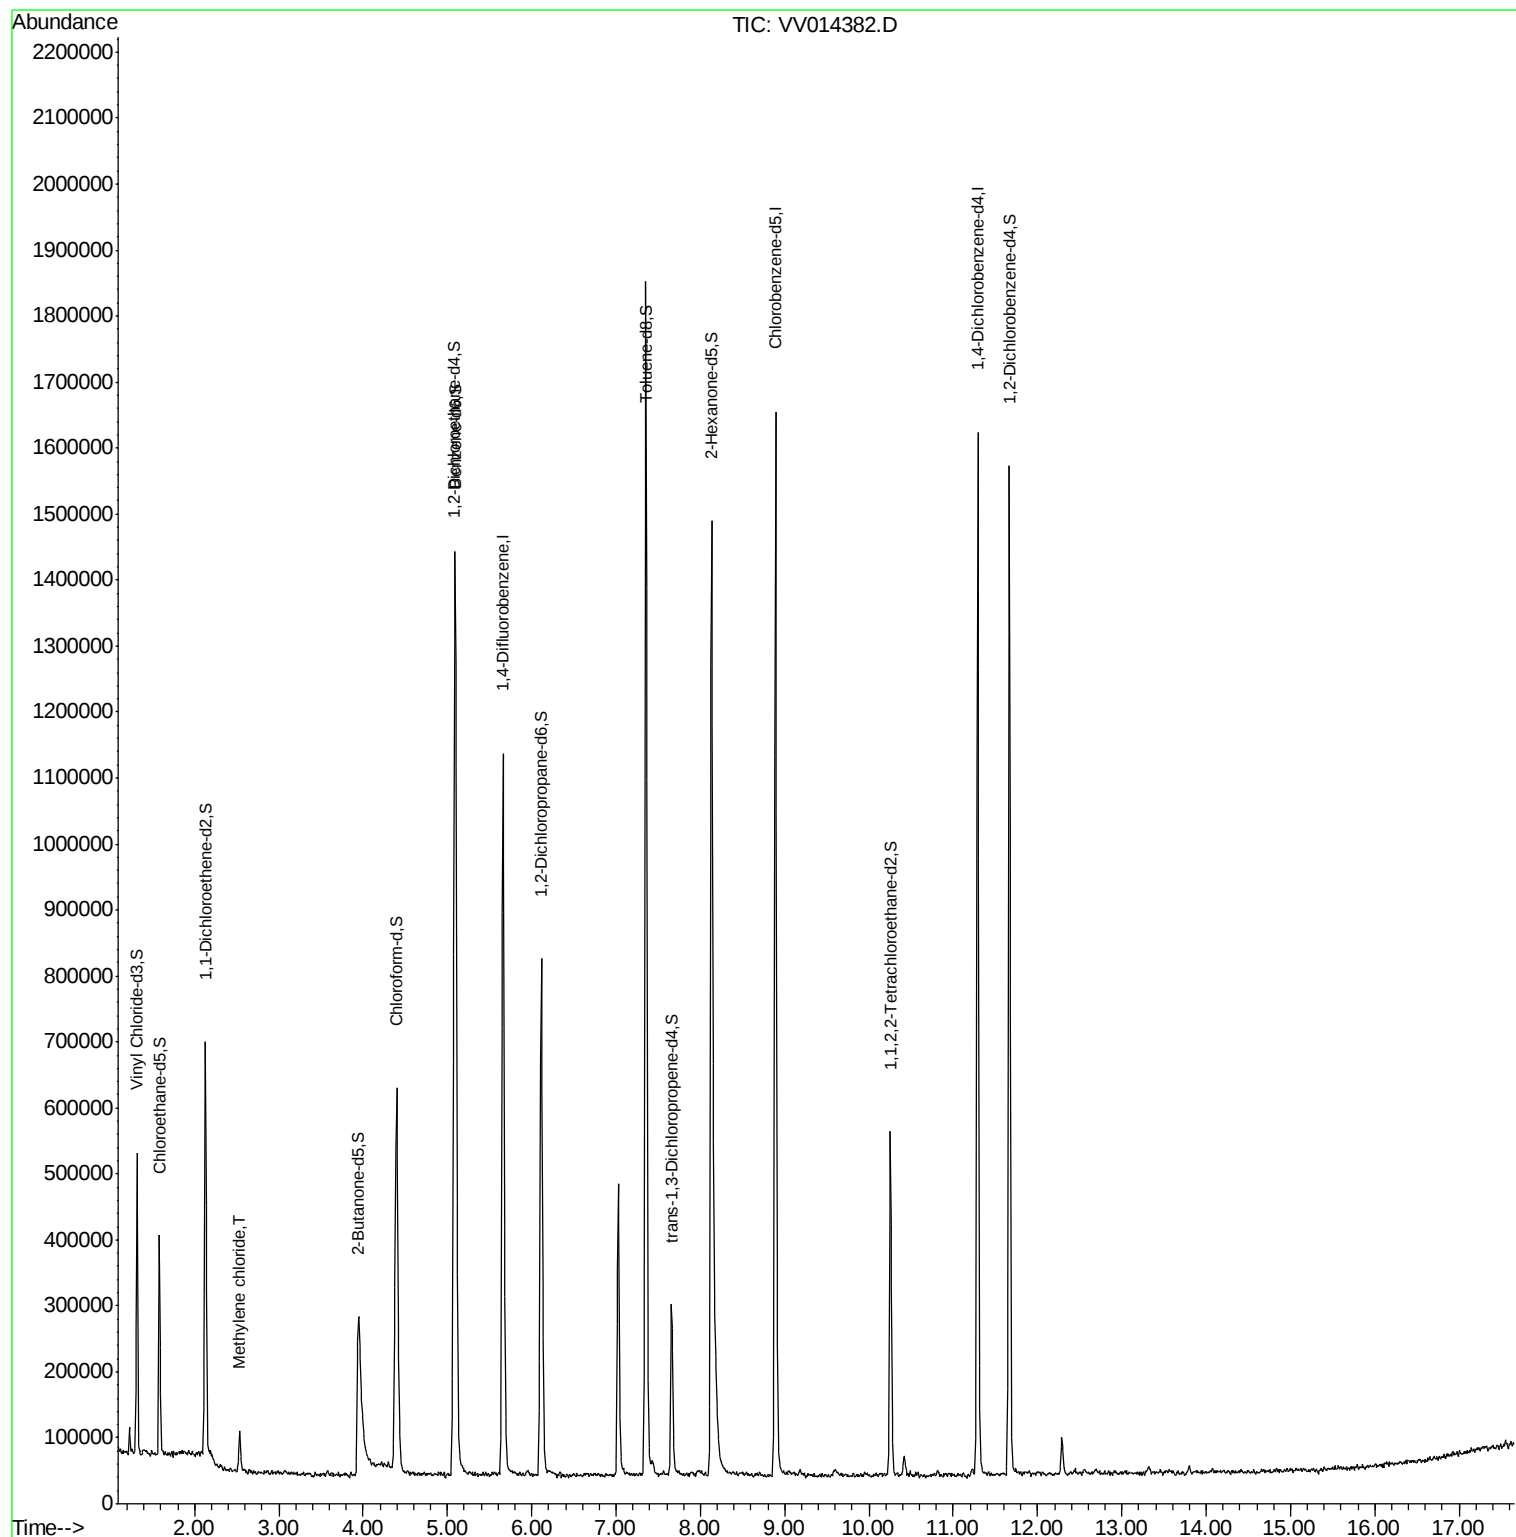

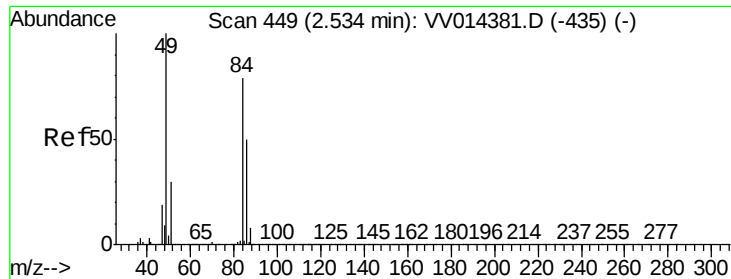

#16
Methylene chloride
Concen: 0.364 ug/L
RT: 2.54 min Scan# 450
Delta R.T. 0.00 min
Lab File: VV014382.D
Acq: 24 Jan 2020 11:46

Instrument :
MSVOA_V
ClientSampleId :
VBLK55

Tot Ion: 84 Resp: 24870
Ion Ratio Lower Upper
84 100
86 70.0 43.1 80.1
49 125.6 82.1 152.5

