




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012423\
 Data File : VV029926.D
 Acq On : 24 Jan 2023 16:28
 Operator : SY/MD
 Sample : 01225-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9H1

Manual IntegrationsAPPROVED

Quant Time: Jan 25 00:45:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 25 00:44:28 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 01/27/2023
 Supervised By :Mahesh Dadoda 01/27/2023

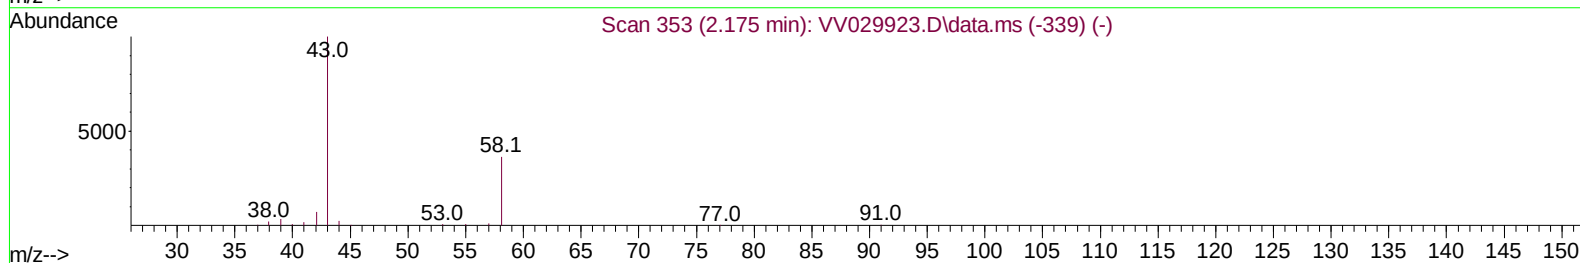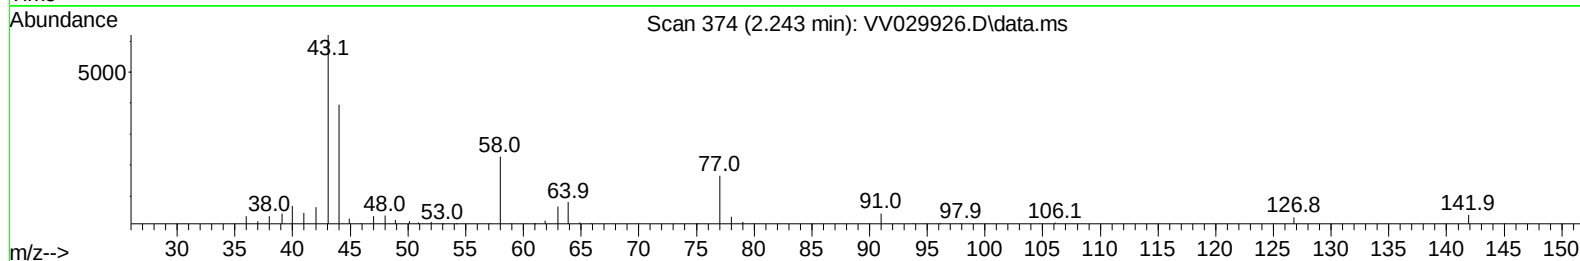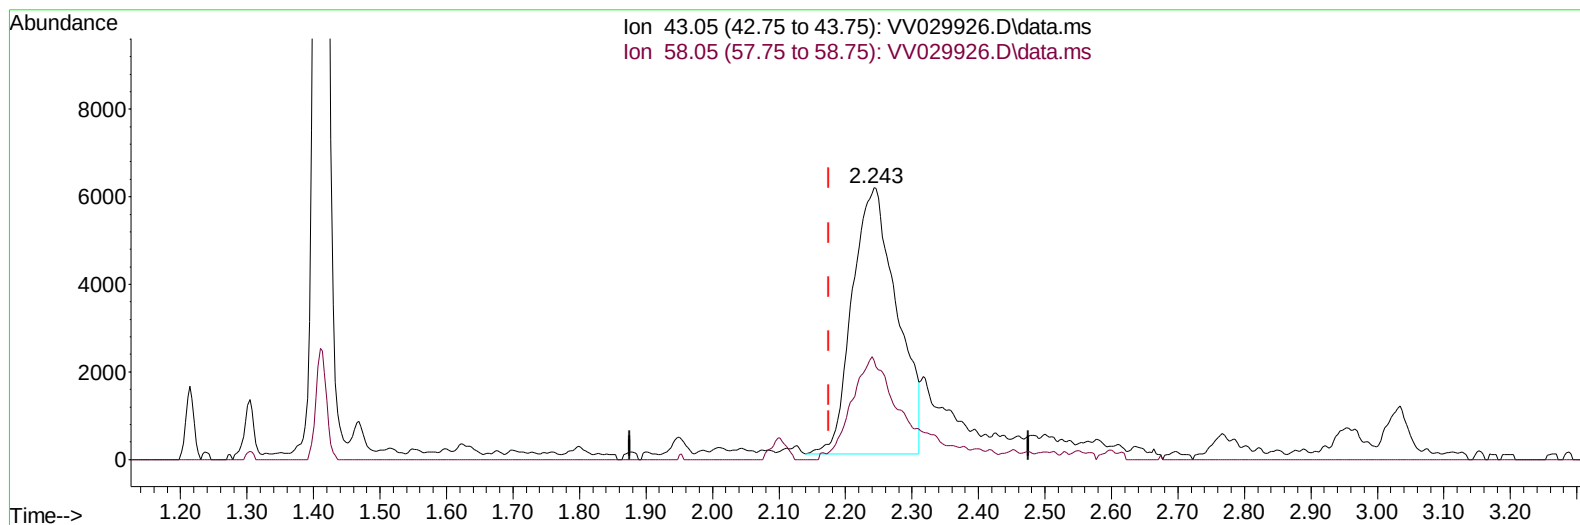

TIC: VV029926.D\data.ms

(13) Acetone (T)

2.243min (+ 0.067) 17.24 ug/L

response 28277

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.40	40.28
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012423\
 Data File : VV029926.D
 Acq On : 24 Jan 2023 16:28
 Operator : SY/MD
 Sample : 01225-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9H1

Manual IntegrationsAPPROVED

Quant Time: Jan 25 00:45:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 25 00:44:28 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 01/27/2023
 Supervised By :Mahesh Dadoda 01/27/2023

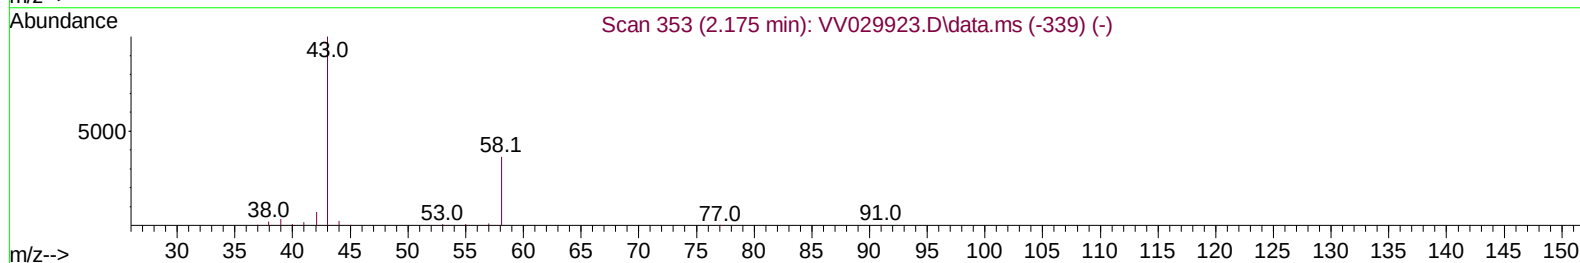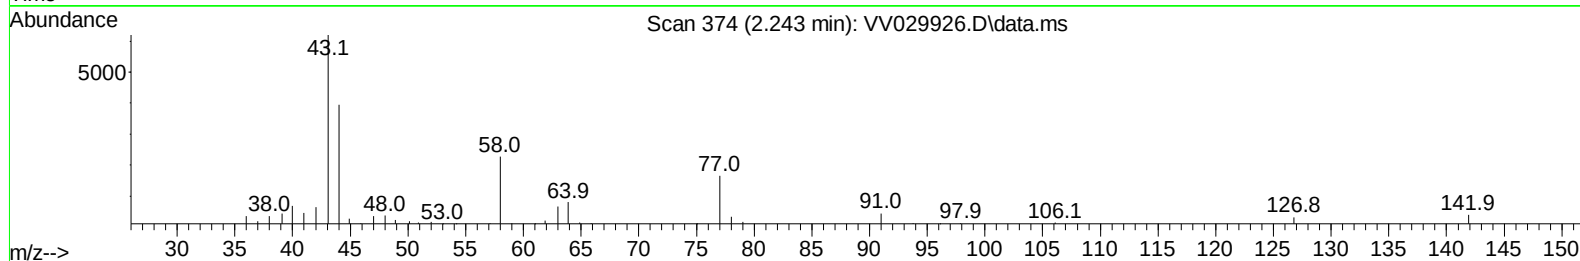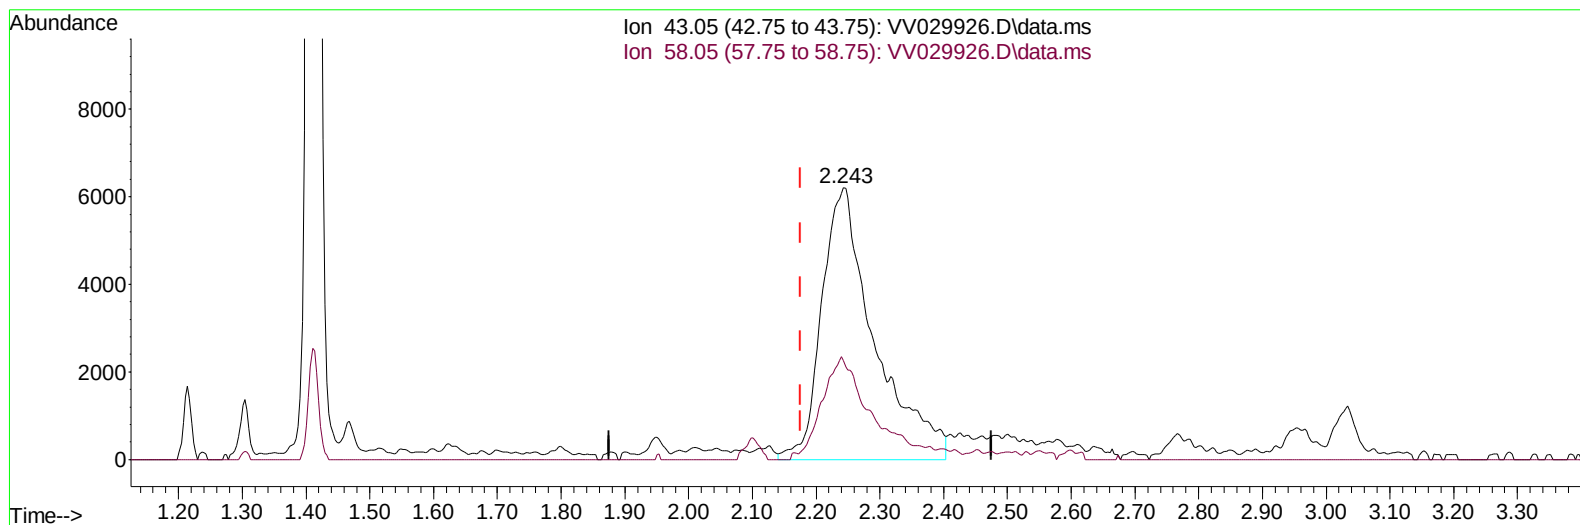

TIC: VV029926.D\data.ms

(13) Acetone (T)

2.243min (+ 0.067) 21.67 ug/L m

response 35553

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.40	32.04
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012423\
 Data File : VV029926.D
 Acq On : 24 Jan 2023 16:28
 Operator : SY/MD
 Sample : 01225-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9H1

Manual IntegrationsAPPROVED

Quant Time: Jan 25 00:45:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 25 00:44:28 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 01/27/2023
 Supervised By :Mahesh Dadoda 01/27/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.606	114		170980	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117		171500	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152		89956	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		67691	5.220	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.400%	
7) Chloroethane-d5	1.564	69		64501	6.000	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	120.000%	
11) 1,1-Dichloroethene-d2	2.101	63		94498	3.997	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.000%	
20) 2-Butanone-d5	3.937	46		107720	46.863	ug/L	0.05
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.720%	
24) Chloroform-d	4.336	84		123444	5.189	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.800%	
26) 1,2-Dichloroethane-d4	5.024	65		51377	5.099	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.000%	
32) Benzene-d6	5.040	84		245004	4.816	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%	
36) 1,2-Dichloropropane-d6	6.059	67		80502	5.407	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.200%	
41) Toluene-d8	7.307	98		201610	4.281	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.600%	
43) trans-1,3-Dichloroprop...	7.616	79		21659	3.983	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.600%	
46) 2-Hexanone-d5	8.088	63		104634	47.267	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.540%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84		57989	5.315	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.200%	
66) 1,2-Dichlorobenzene-d4	11.612	152		82286	5.031	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.600%	
Target Compounds							
						Qvalue	
13) Acetone	2.243	43		35553m	21.671	ug/L	
14) Carbon disulfide	2.285	76		53708	1.278	ug/L	100
16) Methylene chloride	2.500	84		4771	0.263	ug/L	91
17) Methyl tert-butyl Ether	2.767	73		5225	0.207	ug/L #	86
33) Benzene	5.095	78		15285	0.270	ug/L	100
60) Isopropylbenzene	9.921	105		9159	0.159	ug/L #	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012423\
Data File : VV029926.D
Acq On : 24 Jan 2023 16:28
Operator : SY/MD
Sample : 01225-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9H1

Manual IntegrationsAPPROVED

Quant Time: Jan 25 00:45:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 25 00:44:28 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 01/27/2023
Supervised By :Mahesh Dadoda 01/27/2023

