

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012423\
 Data File : VW029928.D
 Acq On : 24 Jan 2023 17:16
 Operator : SY/MD
 Sample : 01225-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9F9

Quant Time: Jan 25 00:46:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 25 00:44:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	172112	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	167920	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	85086	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	66610	5.103	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.000%
7) Chloroethane-d5	1.564	69	64440	5.955	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	119.000%
11) 1,1-Dichloroethene-d2	2.105	63	89838	3.775	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.400%
20) 2-Butanone-d5	3.886	46	116646	50.413	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.820%
24) Chloroform-d	4.339	84	123061	5.139	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.800%
26) 1,2-Dichloroethane-d4	5.024	65	54788	5.402	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.000%
32) Benzene-d6	5.043	84	244001	4.899	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.000%
36) 1,2-Dichloropropane-d6	6.059	67	81327	5.579	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	111.600%
41) Toluene-d8	7.307	98	194061	4.208	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.200%
43) trans-1,3-Dichloroprop...	7.616	79	20544	3.859	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.200%
46) 2-Hexanone-d5	8.085	63	100052	46.160	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.320%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	57121	5.347	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.000%
66) 1,2-Dichlorobenzene-d4	11.612	152	78229	5.057	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.200%
Target Compounds					Qvalue	
13) Acetone	2.175	43	5805	3.515	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012423\
Data File : VV029928.D
Acq On : 24 Jan 2023 17:16
Operator : SY/MD
Sample : 01225-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9F9

Quant Time: Jan 25 00:46:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 25 00:44:28 2023
Response via : Initial Calibration

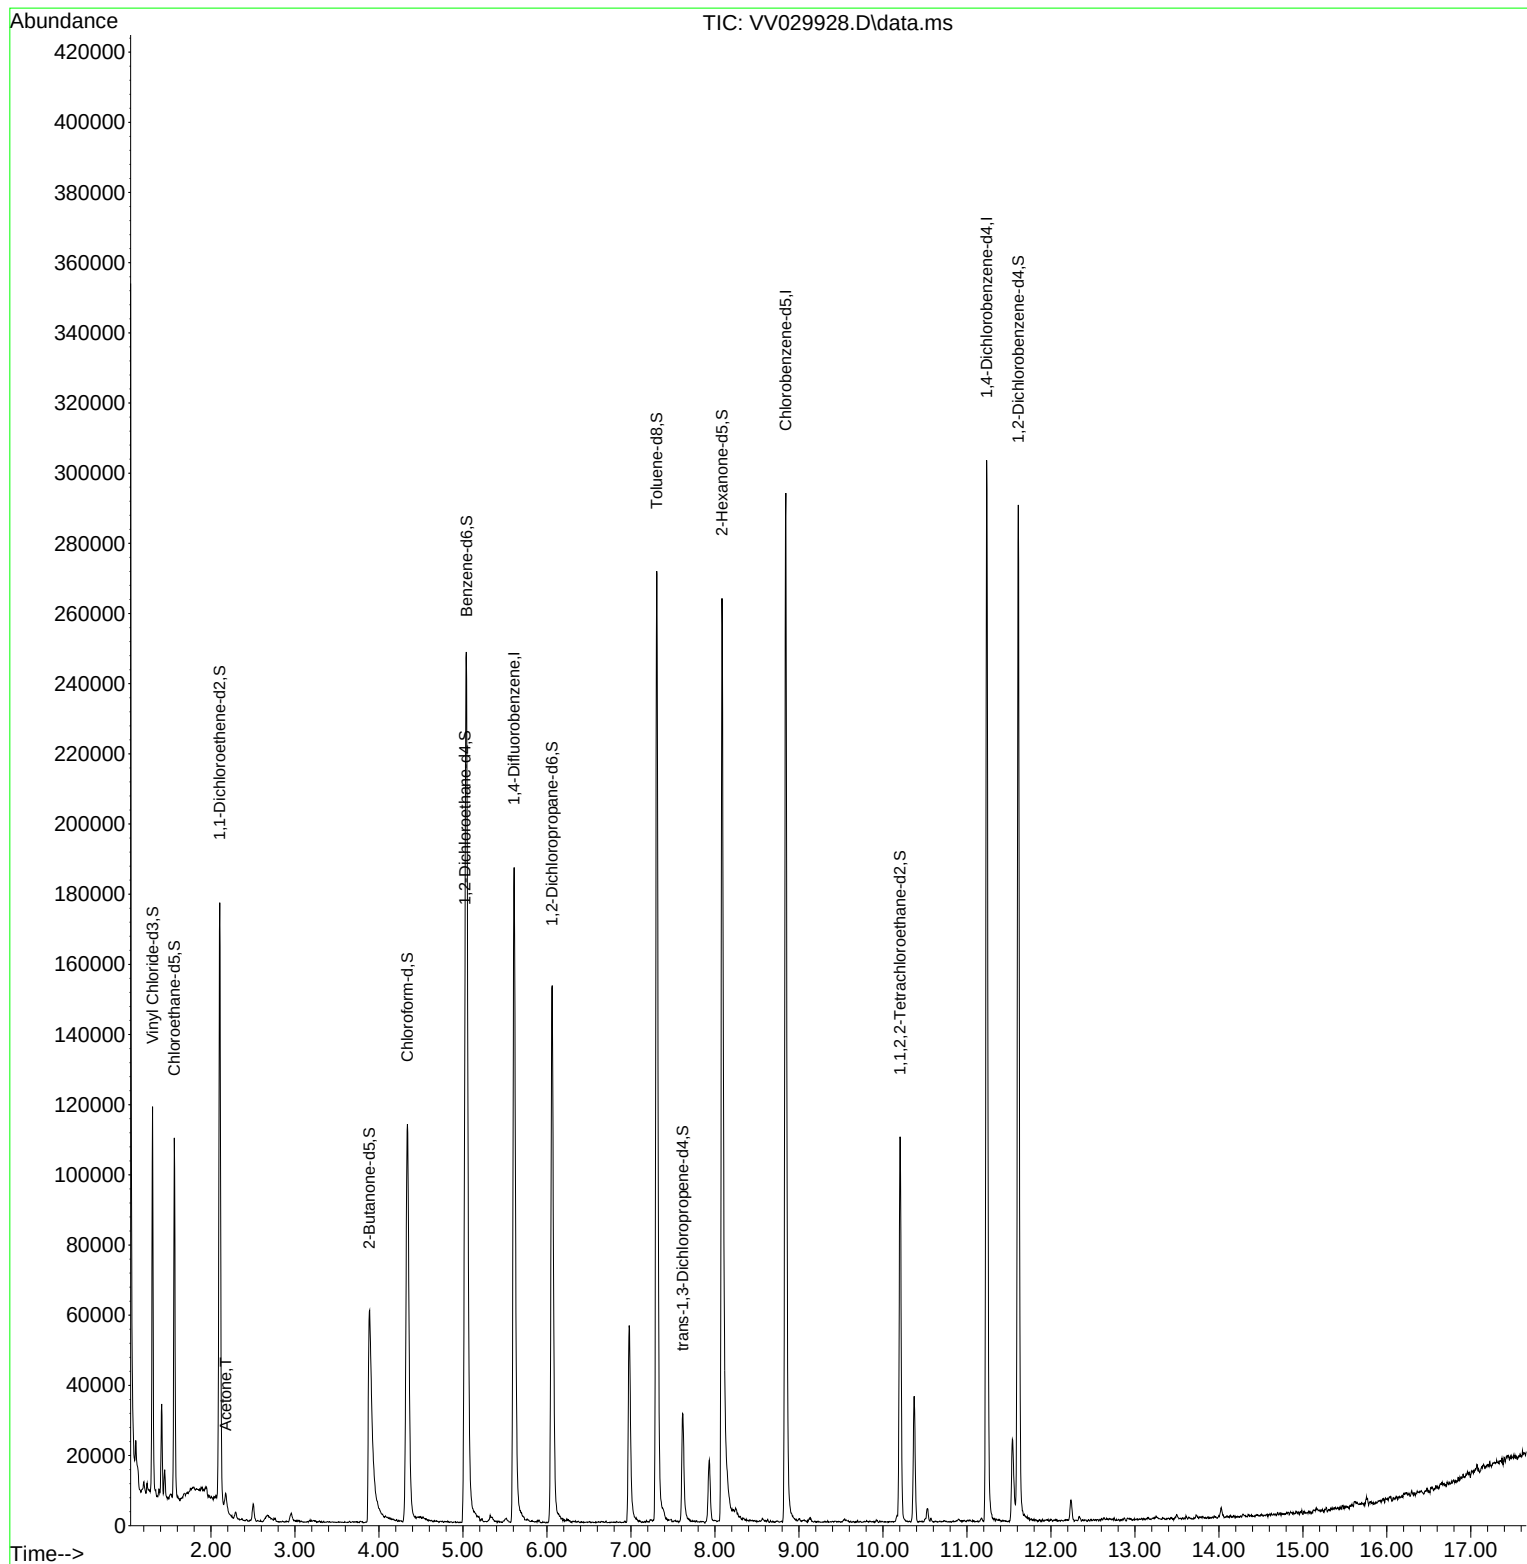

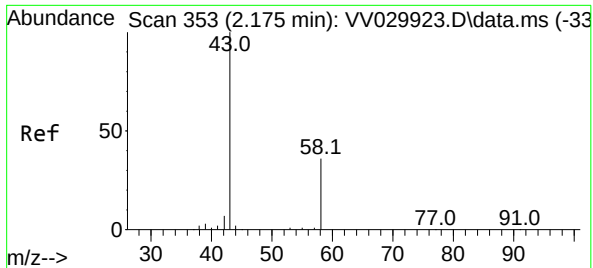

#13
 Acetone
 Concen: 3.515 ug/L
 RT: 2.175 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VV029928.D
 Acq: 24 Jan 2023 17:16

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9F9

Tgt Ion: 43 Resp: 5805
 Ion Ratio Lower Upper
 43 100
 58 43.1 0.0 68.8

