

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012423\
 Data File : VV029927.D
 Acq On : 24 Jan 2023 16:52
 Operator : SY/MD
 Sample : 01225-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9G0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	22	29	38	rVB	208697	204431	32.04%	3.599%
2	1.304	74	82	96	rVB	110076	116510	18.26%	2.051%
3	1.410	108	115	123	rBV	107366	120891	18.95%	2.128%
4	1.445	123	126	136	rVB4	6403	6843	1.07%	0.120%
5	1.564	155	163	174	rVB	102771	113942	17.86%	2.006%
6	2.101	320	330	350	rVB	177054	264566	41.47%	4.658%
7	2.500	446	454	465	rVB4	4500	7864	1.23%	0.138%
8	3.921	880	896	940	rBV3	41988	207621	32.54%	3.655%
9	4.339	1009	1026	1056	rBV	109717	278601	43.67%	4.905%
10	5.040	1227	1244	1276	rBV2	253541	637964	100.00%	11.232%
11	5.609	1406	1421	1448	rBV	195431	408599	64.05%	7.194%
12	6.063	1548	1562	1589	rBV	149427	317314	49.74%	5.587%
13	6.979	1832	1847	1865	rBV	56238	108646	17.03%	1.913%
14	7.307	1935	1949	1986	rBV	275912	500711	78.49%	8.816%
15	7.616	2036	2045	2061	rBV	32074	58704	9.20%	1.034%
16	7.931	2131	2143	2160	rBV2	22998	41736	6.54%	0.735%
17	8.088	2182	2192	2235	rBV	251629	546314	85.63%	9.618%
18	8.844	2416	2427	2453	rBV	293312	497005	77.90%	8.750%
19	10.207	2840	2851	2866	rVB	105820	168716	26.45%	2.970%
20	10.371	2891	2902	2917	rVB	51788	86788	13.60%	1.528%
21	11.236	3160	3171	3194	rBV	306451	487154	76.36%	8.577%
22	11.545	3257	3267	3276	rBV3	11411	21711	3.40%	0.382%
23	11.612	3277	3288	3305	rVB	278205	439976	68.97%	7.746%
24	12.239	3470	3483	3493	rVB	13480	22187	3.48%	0.391%
25	14.027	4029	4039	4047	rBV2	4703	8253	1.29%	0.145%
26	14.284	4110	4119	4129	rBV10	3355	6795	1.07%	0.120%


Sum of corrected areas: 5679842

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012423\
Data File : VV029927.D
Acq On : 24 Jan 2023 16:52
Operator : SY/MD
Sample : 01225-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9G0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

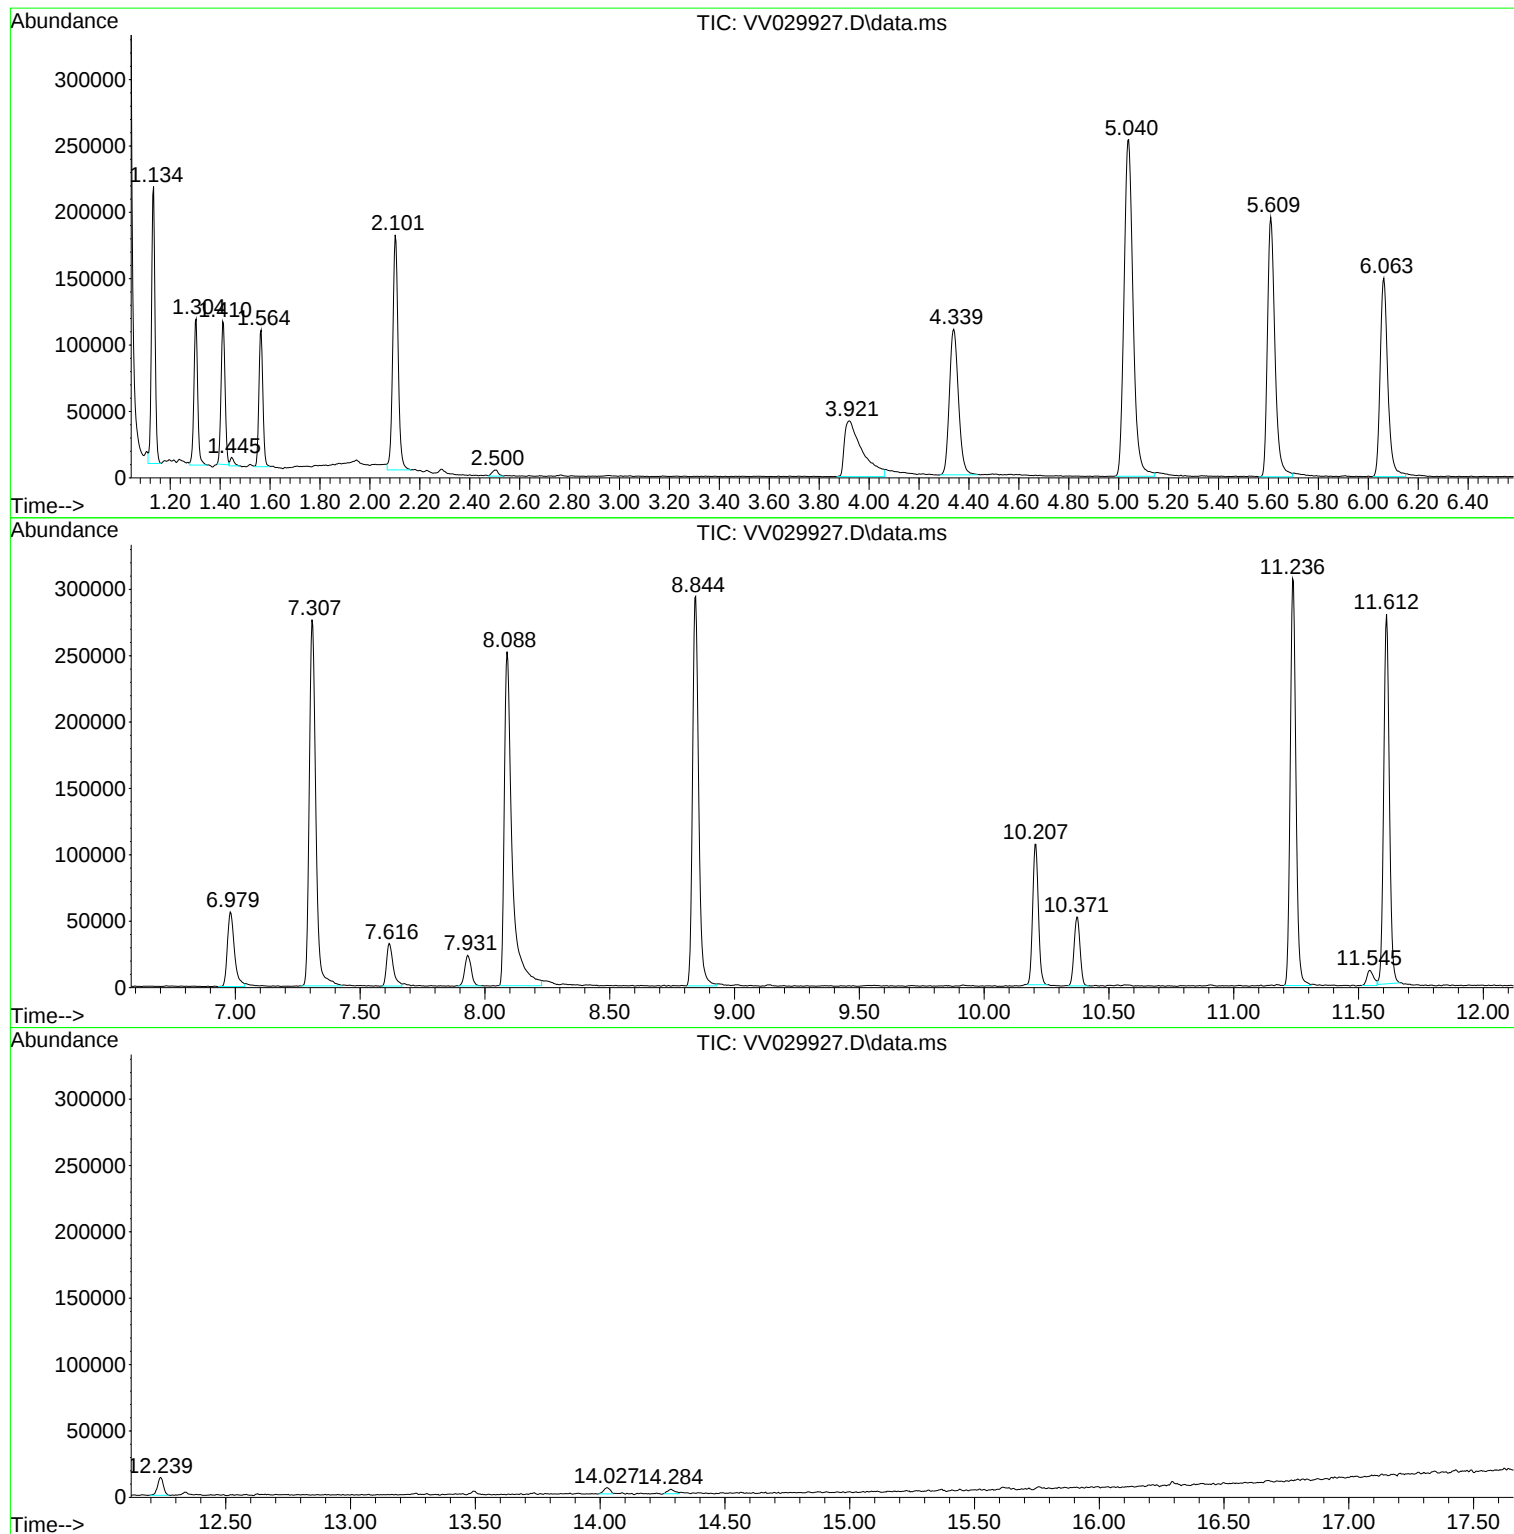

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012423\
Data File : VV029927.D
Acq On : 24 Jan 2023 16:52
Operator : SY/MD
Sample : 01225-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9G0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012423\
Data File : VV029927.D
Acq On : 24 Jan 2023 16:52
Operator : SY/MD
Sample : 01225-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9G0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc