
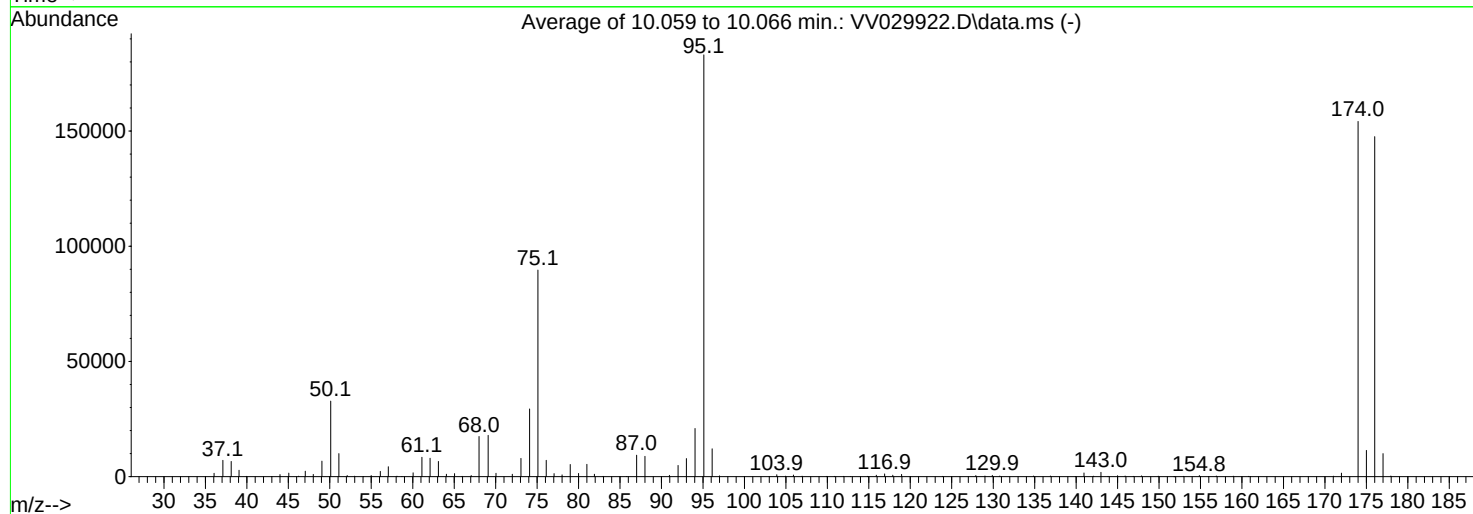


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012423\
Data File : VV029922.D
Acq On : 24 Jan 2023 13:00
Operator : SY/MD
Sample : BFB215
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB215

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jan 27 01:28:41 2023

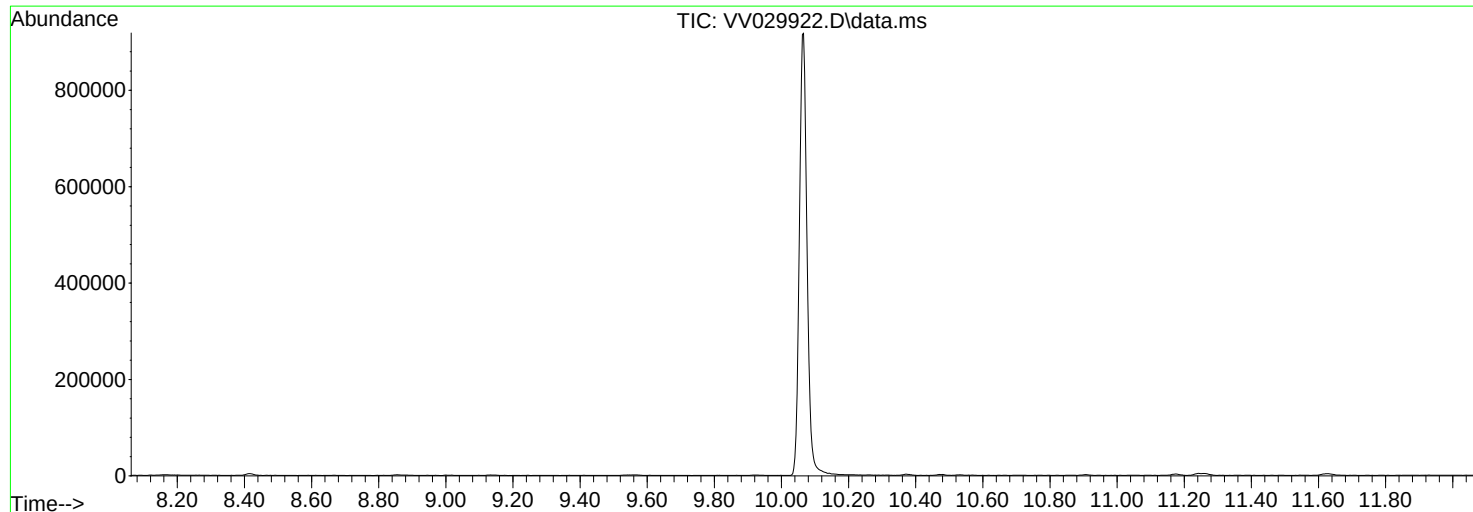

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2793

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	32755	PASS
75	95	30	80	49.0	89669	PASS
95	95	100	100	100.0	183061	PASS
96	95	5	9	6.6	12056	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.2	154176	PASS
175	174	5	9	7.4	11366	PASS
176	174	95	105	95.7	147563	PASS
177	176	5	10	6.8	10004	PASS

m/z	Abundance
40.00	364.0
43.00	104.0
44.00	650.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
36.10	1466.0
37.10	6834.0
38.10	6489.0
39.00	2733.0
39.90	495.0
43.00	148.0
44.00	1603.0
45.10	1433.0
46.30	231.0
47.10	2293.0
48.00	901.0
49.00	6469.0
50.10	30856.0
51.10	9638.0
52.10	512.0
53.00	244.0
54.10	107.0
55.00	463.0
56.10	2166.0
57.10	4129.0
58.10	222.0
58.70	100.0
60.10	1563.0
61.10	8036.0
62.10	7562.0
63.10	6387.0
64.00	933.0
65.00	1256.0
66.00	161.0
67.00	511.0
68.00	16512.0
69.10	16856.0
70.10	1355.0
72.00	998.0
73.10	7604.0
74.10	27552.0
75.10	84872.0
76.10	6910.0
77.00	1199.0
78.00	760.0
79.00	4953.0
80.00	1314.0
81.00	4928.0
81.90	929.0
83.00	112.0
85.80	213.0
87.00	8433.0
88.00	8240.0
90.90	582.0
92.00	4546.0
93.00	7189.0
94.00	19560.0
95.10	171520.0
96.10	11150.0
97.00	419.0
103.00	104.0
103.90	805.0
104.90	179.0
105.90	691.0
107.00	188.0
109.90	149.0
110.80	141.0
112.00	127.0
112.80	121.0
114.80	145.0
115.90	572.0
116.90	1174.0
117.90	613.0
119.00	917.0
123.90	103.0
127.90	486.0
129.10	323.0
129.90	582.0
130.80	269.0
134.80	278.0
136.90	221.0
141.00	1415.0
142.10	201.0
143.00	1839.0
143.90	143.0
145.00	387.0
145.90	265.0
146.90	118.0
147.90	332.0
149.90	164.0
152.90	128.0
154.80	459.0
156.90	309.0
159.00	190.0
160.80	219.0
171.00	229.0
172.00	1370.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

174.00	140416.0
175.00	10606.0
176.00	133056.0
177.00	9431.0
177.90	251.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
36.10	1501.0
37.10	7302.0
38.10	6823.0
39.10	2839.0
39.90	498.0
43.00	154.0
44.10	1612.0
45.10	1623.0
46.30	246.0
47.10	2403.0
48.00	1047.0
49.10	6907.0
50.10	34000.0
51.10	10384.0
52.10	544.0
53.00	227.0
54.00	103.0
55.00	496.0
56.10	2342.0
57.10	4435.0
58.10	243.0
58.70	124.0
60.00	1735.0
61.10	8608.0
62.10	8263.0
63.10	6752.0
64.00	1043.0
65.00	1377.0
66.00	162.0
67.10	526.0
68.00	18160.0
69.10	18488.0
70.10	1537.0
72.00	1057.0
73.00	8190.0
74.10	30144.0
75.10	92728.0
76.10	7317.0
77.10	1364.0
78.00	786.0
79.00	5446.0
80.00	1477.0
81.00	5520.0
81.90	1079.0
82.90	127.0
87.00	9631.0
88.00	9160.0
91.00	620.0
92.00	4965.0
93.00	8092.0
94.10	21592.0
95.10	189312.0
96.10	12469.0
97.00	363.0
103.00	111.0
103.90	845.0
105.00	200.0
105.90	765.0
106.90	217.0
109.90	169.0
110.80	167.0
111.90	121.0
112.80	119.0
114.90	153.0
115.90	632.0
116.90	1232.0
117.90	672.0
118.90	968.0
123.90	138.0
127.90	538.0
129.00	304.0
129.90	629.0
130.80	284.0
134.80	303.0
136.90	288.0
139.90	121.0
141.00	1687.0
142.10	211.0
143.00	1966.0
143.80	143.0
145.00	441.0
145.90	287.0
146.90	158.0
147.90	398.0
149.90	198.0
153.00	156.0
154.80	472.0
156.00	102.0
156.90	288.0
158.90	213.0
160.80	186.0
171.00	233.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

172.00	1551.0
174.00	159168.0
175.00	11723.0
176.00	152384.0
177.00	10312.0
178.00	258.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
36.00	1399.0
37.10	7073.0
38.10	6592.0
39.10	2794.0
40.00	495.0
43.00	149.0
44.10	1558.0
45.00	1586.0
46.20	234.0
47.00	2342.0
48.00	1087.0
49.10	6824.0
50.10	33408.0
51.10	10053.0
52.10	514.0
53.00	196.0
55.00	488.0
56.10	2350.0
57.00	4279.0
58.10	216.0
60.00	1697.0
61.10	8663.0
62.10	8181.0
63.10	6623.0
64.10	1079.0
65.10	1407.0
65.90	136.0
67.10	528.0
68.00	17728.0
69.10	18488.0
70.00	1462.0
72.00	1011.0
73.00	7963.0
74.10	30376.0
75.10	91408.0
76.10	7058.0
77.10	1409.0
78.00	756.0
79.00	5435.0
80.00	1396.0
81.00	5577.0
81.90	1078.0
82.90	127.0
87.00	9905.0
88.00	9067.0
91.00	565.0
92.00	5028.0
93.00	8326.0
94.10	21552.0
95.10	188352.0
96.10	12550.0
97.00	303.0
103.90	793.0
105.00	196.0
105.90	735.0
106.90	209.0
110.00	158.0
110.90	167.0
111.90	115.0
114.90	162.0
115.90	661.0
116.90	1171.0
117.90	656.0
118.90	962.0
123.90	133.0
127.90	558.0
128.90	317.0
129.90	585.0
130.80	256.0
134.90	292.0
136.90	331.0
139.90	138.0
140.90	1759.0
142.10	172.0
143.00	1929.0
143.80	116.0
145.00	434.0
145.90	291.0
146.90	159.0
147.90	403.0
149.90	208.0
151.80	106.0
153.00	174.0
154.90	465.0
156.00	140.0
156.90	274.0
158.90	216.0
161.00	149.0
171.10	212.0
172.00	1705.0
174.00	162944.0
175.00	11768.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

176.00157248.0

177.0010270.0

178.00250.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215