
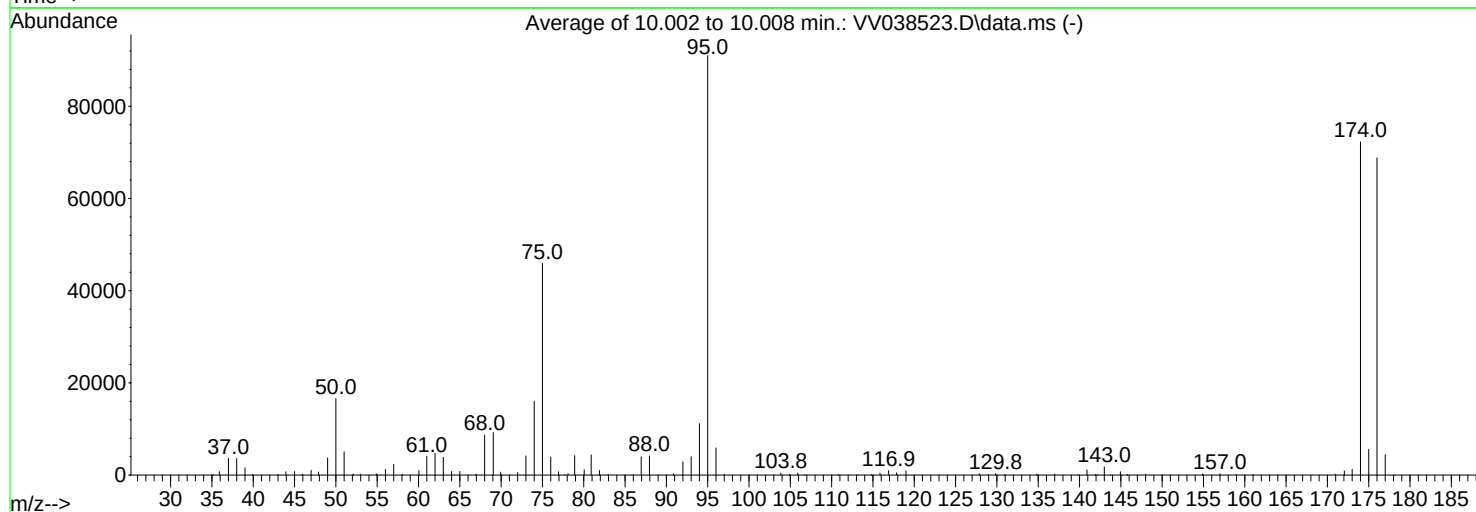


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV012425\
Data File : VV038523.D
Acq On : 24 Jan 2025 08:39
Operator : SY/MD
Sample : BFB402
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB402

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011725WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 30 08:15:13 2025

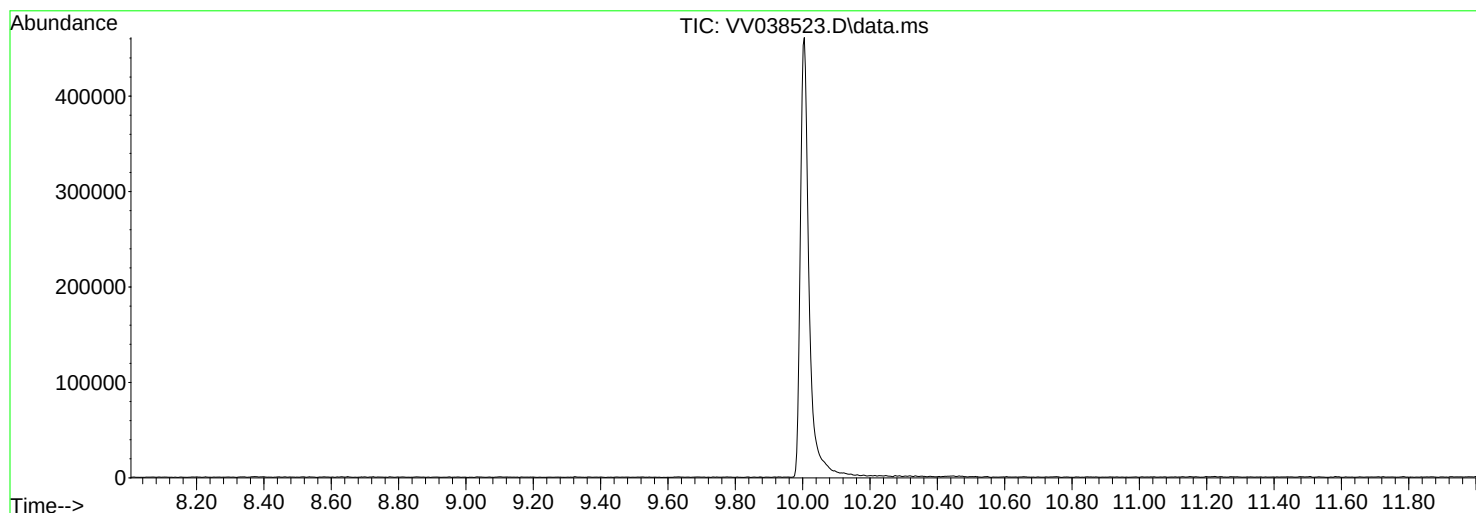

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	16556	PASS
75	95	30	80	50.5	45915	PASS
95	95	100	100	100.0	90971	PASS
96	95	5	9	6.5	5893	PASS
173	174	0.00	2	1.8	1298	PASS
174	95	50	120	79.5	72291	PASS
175	174	5	9	7.7	5583	PASS
176	174	95	105	95.2	68789	PASS
177	176	5	10	6.5	4451	PASS

m/z	Abundance
39.90	399.0
44.20	283.0

Instrument :
MSVOA_V
ClientSampleId :
BFB402

m/z	Abundance
35.20	126.0
35.90	778.0
37.00	3752.0
38.00	3813.0
39.00	1586.0
40.00	559.0
43.00	116.0
43.90	746.0
45.00	763.0
45.90	252.0
47.00	1085.0
47.90	617.0
49.00	3626.0
50.00	17048.0
51.00	4919.0
52.10	311.0
53.00	193.0
54.90	247.0
56.00	1172.0
57.00	2359.0
58.10	179.0
60.10	948.0
61.00	4131.0
62.00	4812.0
63.00	3852.0
64.00	708.0
65.00	806.0
67.00	190.0
68.00	9154.0
69.00	9501.0
69.90	649.0
72.00	531.0
73.00	4315.0
74.00	16232.0
75.00	47192.0
76.00	4135.0
77.00	694.0
78.00	339.0
78.90	4421.0
80.00	1106.0
80.90	4520.0
81.90	1113.0
82.90	117.0
87.00	4008.0
87.90	4271.0
90.90	355.0
92.00	2623.0
93.00	3861.0
94.00	11658.0
95.00	93152.0
96.00	6288.0
97.00	225.0
103.80	423.0
104.90	175.0
105.90	461.0
110.80	142.0
115.00	103.0
115.90	425.0
116.90	1005.0
117.80	568.0
119.00	884.0
127.90	357.0
128.90	185.0
129.80	387.0
130.90	117.0
134.80	253.0
136.90	254.0
139.90	125.0
140.90	1150.0
141.90	161.0
142.20	153.0
143.00	1782.0
143.80	171.0
145.00	750.0
145.90	152.0
148.00	218.0
154.90	224.0
157.00	298.0
159.00	108.0
170.90	231.0
172.10	858.0
173.00	1163.0
174.00	70944.0
175.00	5551.0
176.00	68952.0
177.00	4278.0
178.20	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB402

m/z	Abundance
35.20	139.0
35.90	780.0
37.00	3724.0
38.00	3754.0
39.00	1609.0
39.90	475.0
43.00	153.0
43.90	713.0
45.00	788.0
45.90	210.0
47.00	1037.0
47.90	698.0
49.00	3852.0
50.00	17112.0
51.00	5227.0
52.10	251.0
52.90	222.0
54.90	270.0
56.00	1230.0
57.00	2415.0
58.00	181.0
60.10	965.0
61.00	4223.0
62.00	4935.0
63.00	4021.0
64.00	796.0
65.00	853.0
67.00	233.0
68.00	8753.0
69.10	9449.0
70.00	668.0
72.00	583.0
73.00	4275.0
74.00	16520.0
75.00	47144.0
76.00	3948.0
76.90	662.0
78.10	291.0
78.90	4313.0
80.00	1174.0
80.90	4550.0
81.90	1063.0
83.00	159.0
87.00	4027.0
88.00	4305.0
90.80	328.0
92.00	2884.0
93.00	4075.0
94.00	11409.0
95.00	93808.0
96.00	6066.0
97.10	161.0
103.90	487.0
104.90	183.0
105.90	480.0
106.70	110.0
110.80	144.0
114.80	142.0
115.90	414.0
116.90	1044.0
117.80	505.0
119.00	975.0
127.80	303.0
129.00	170.0
129.90	362.0
130.90	115.0
134.80	263.0
137.00	229.0
139.70	101.0
140.90	1173.0
141.90	192.0
143.00	1875.0
143.70	131.0
144.90	735.0
145.80	171.0
148.00	230.0
154.90	287.0
157.00	291.0
158.90	152.0
161.00	118.0
170.90	220.0
172.00	946.0
173.00	1379.0
174.00	74520.0
175.00	5735.0
176.00	71024.0
177.00	4610.0

Instrument :
MSVOA_V
ClientSampleId :
BFB402

m/z	Abundance
35.90	704.0
37.00	3525.0
38.00	3229.0
39.00	1523.0
39.90	394.0
43.00	145.0
44.00	694.0
45.00	726.0
46.00	157.0
47.00	962.0
47.90	670.0
49.00	3708.0
50.00	15507.0
51.00	5030.0
52.10	189.0
52.90	246.0
54.90	293.0
56.00	1303.0
57.00	2187.0
58.00	153.0
60.00	983.0
61.00	3998.0
62.00	4477.0
63.00	3748.0
64.00	787.0
65.00	734.0
66.90	303.0
68.00	8161.0
69.10	8767.0
70.00	613.0
72.00	550.0
73.00	3894.0
74.00	15239.0
75.00	43408.0
76.00	3660.0
76.90	759.0
77.70	185.0
78.20	298.0
78.90	3940.0
80.10	1153.0
80.90	4128.0
81.90	863.0
83.00	197.0
86.00	160.0
86.90	3760.0
88.00	3878.0
90.80	316.0
92.00	3115.0
93.00	4041.0
94.00	10402.0
95.00	85952.0
96.00	5326.0
97.00	134.0
103.90	474.0
104.90	161.0
105.90	422.0
106.80	144.0
110.80	144.0
113.20	133.0
114.70	168.0
115.80	425.0
116.90	893.0
117.90	407.0
119.00	893.0
127.90	280.0
128.90	177.0
129.90	358.0
131.00	137.0
134.90	218.0
137.10	190.0
140.90	1052.0
141.90	167.0
143.00	1715.0
144.90	703.0
145.70	202.0
148.00	181.0
154.90	270.0
157.00	217.0
158.90	148.0
161.00	139.0
171.00	213.0
172.00	888.0
173.00	1352.0
174.00	71408.0
175.00	5462.0
176.00	66392.0
177.00	4464.0

Instrument :
MSVOA_V
ClientSampleId :
BFB402