

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012521\
 Data File : VV020155.D
 Acq On : 25 Jan 2021 12:04
 Operator : SY/MD
 Sample : M1199-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jan 25 15:32:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 25 15:30:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	388659	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.859	117	408116	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.254	152	228611	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.309	65	150448	52.19	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 104.38%			
7) Chloroethane-d5	1.569	69	130638	54.14	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 108.28%			
11) 1,1-Dichloroethene-d2	2.110	63	229339	39.83	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 79.66%			
21) 2-Butanone-d5	3.888	46	201531	101.94	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 101.94%			
24) Chloroform-d	4.354	84	271344	50.25	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.50%			
26) 1,2-Dichloroethane-d4	5.036	65	195453	52.22	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 104.44%			
32) Benzene-d6	5.055	84	510226	45.40	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 90.80%			
36) 1,2-Dichloropropane-d6	6.074	67	164001	46.22	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 92.44%			
41) Toluene-d8	7.318	98	522303	49.95	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 99.90%			
43) trans-1,3-Dichloroprop...	7.624	79	74724	43.04	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 86.08%			
47) 2-Hexanone-d5	8.093	63	111856	75.84	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 75.84%			
57) 1,1,2,2-Tetrachloroeth...	10.222	84	215113	44.29	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 88.58%			
64) 1,2-Dichlorobenzene-d4	11.630	152	180307	41.97	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 83.94%			
Target Compounds					Qvalue	
48) 2-Hexanone	8.145	43	11076	2.98	ug/L #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012521\
Data File : VV020155.D
Acq On : 25 Jan 2021 12:04
Operator : SY/MD
Sample : M1199-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jan 25 15:32:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 25 15:30:53 2021
Response via : Initial Calibration

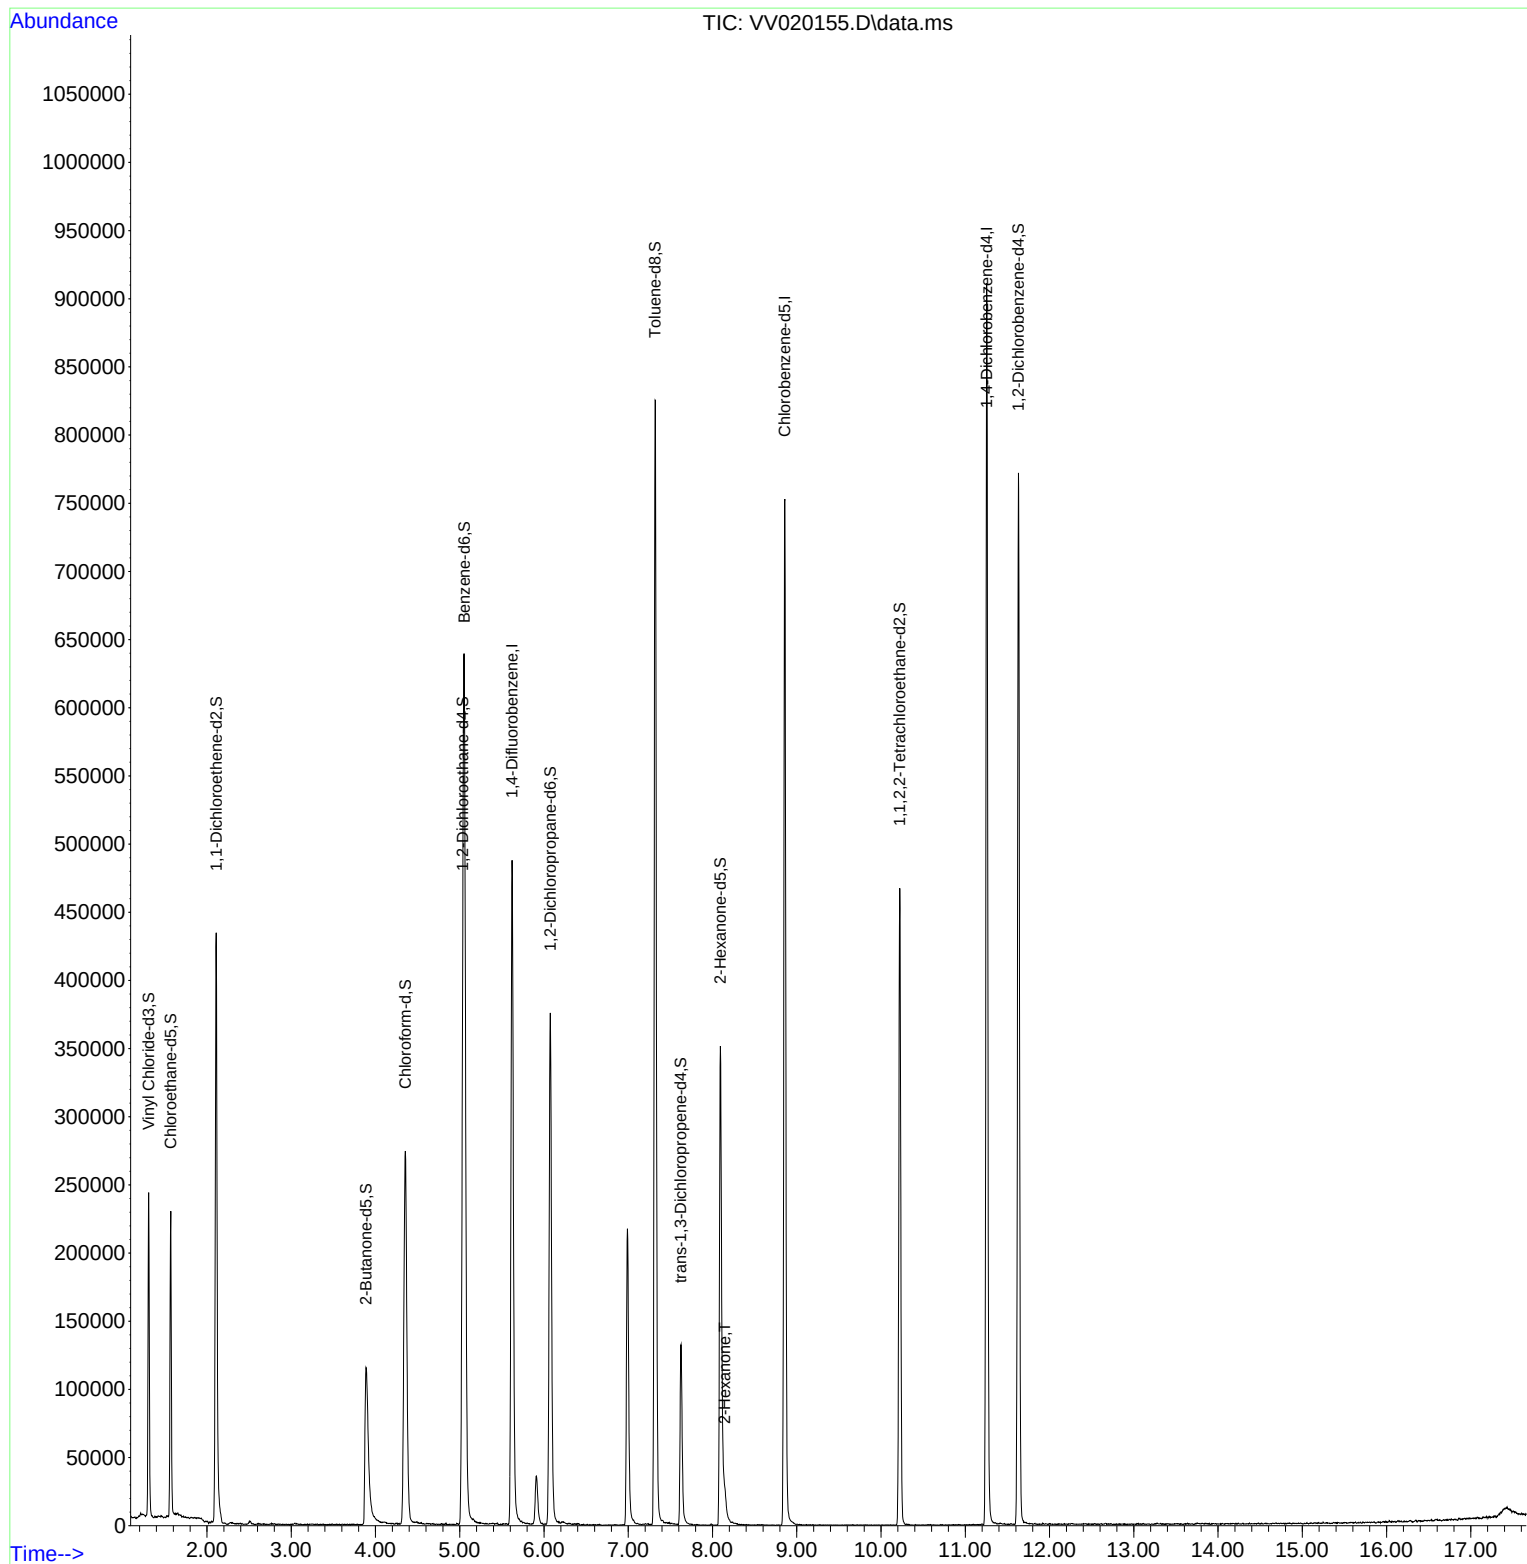

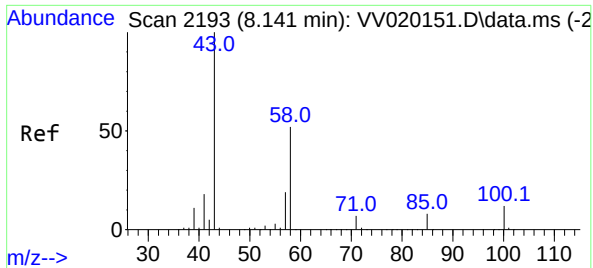

#48
2-Hexanone
Concen: 2.98 ug/L
RT: 8.145 min Scan# 2194
Delta R.T. 0.003 min
Lab File: VV020155.D
Acq: 25 Jan 2021 12:04

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Tgt Ion: 43	Resp: 11076
Ion Ratio	Lower Upper
43	100
58	45.2 41.8 62.6
57	0.9 15.0 22.4#
100	11.4 8.9 13.3

