

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012521\
 Data File : VV020152.D
 Acq On : 25 Jan 2021 10:53
 Operator : SY/MD
 Sample : VV0125WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

Signal : TIC: VV020152.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	86	rVB	236407	242213	15.46%	1.908%
2	1.570	142	149	161	rVB	217928	235280	15.02%	1.853%
3	2.110	307	317	343	rVB	433241	654638	41.78%	5.157%
4	2.592	465	467	469	rVB2	923	336	0.02%	0.003%
5	2.611	469	473	474	rBV3	679	499	0.03%	0.004%
6	2.730	508	510	511	rBV	569	280	0.02%	0.002%
7	2.788	526	528	529	rBV	640	308	0.02%	0.002%
8	2.840	541	544	550	rVB5	805	814	0.05%	0.006%
9	2.885	555	558	560	rBV2	484	344	0.02%	0.003%
10	3.061	610	613	616	rVB	788	334	0.02%	0.003%
11	3.081	616	619	621	rBV2	672	378	0.02%	0.003%
12	3.164	642	645	647	rBV2	317	247	0.02%	0.002%
13	3.296	684	686	688	rBV	367	232	0.01%	0.002%
14	3.354	701	704	705	rBV2	353	227	0.01%	0.002%
15	3.386	712	714	716	rBV	531	249	0.02%	0.002%
16	3.402	716	719	722	rVB3	783	356	0.02%	0.003%
17	3.463	735	738	741	rBV3	745	481	0.03%	0.004%
18	3.528	753	758	760	rBV3	621	580	0.04%	0.005%
19	3.586	773	776	780	rBV3	718	428	0.03%	0.003%
20	3.643	792	794	797	rVB	600	335	0.02%	0.003%
21	3.885	859	869	907	rBV	106013	313692	20.02%	2.471%
22	4.351	997	1014	1039	rBV	256075	637872	40.71%	5.025%
23	4.756	1137	1140	1141	rBV2	479	269	0.02%	0.002%
24	4.852	1166	1170	1173	rVB4	469	313	0.02%	0.002%
25	4.930	1190	1194	1200	rVB5	770	758	0.05%	0.006%
26	4.958	1200	1203	1207	rVB4	620	468	0.03%	0.004%
27	4.978	1207	1209	1211	rBV	868	399	0.03%	0.003%
28	5.048	1211	1231	1260	rBV2	603764	1566691	100.00%	12.341%
29	5.438	1348	1352	1353	rBV3	687	497	0.03%	0.004%
30	5.618	1395	1408	1439	rBV	481943	969251	61.87%	7.635%
31	5.910	1488	1499	1519	rVB3	33166	69162	4.41%	0.545%
32	6.071	1532	1549	1575	rBV	358829	739759	47.22%	5.827%
33	6.299	1617	1620	1622	rBV3	768	432	0.03%	0.003%
34	6.341	1630	1633	1634	rBV2	400	195	0.01%	0.002%
35	6.364	1638	1640	1642	rVV3	545	190	0.01%	0.001%
36	6.415	1654	1656	1663	rVB4	645	462	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012521\
 Data File : VV020152.D
 Acq On : 25 Jan 2021 10:53
 Operator : SY/MD
 Sample : VV0125WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis

37	6.444	1663	1665	1666	rBV	368	187	0.01%	0.001%
38	6.489	1677	1679	1683	rVB2	711	484	0.03%	0.004%
39	6.540	1687	1695	1697	rBV4	843	826	0.05%	0.007%
40	6.569	1701	1704	1707	rBV3	373	245	0.02%	0.002%
41	6.688	1739	1741	1743	rBV2	427	202	0.01%	0.002%
42	6.733	1752	1755	1757	rBV2	434	260	0.02%	0.002%
43	6.759	1760	1763	1767	rVB3	693	569	0.04%	0.004%
44	6.788	1767	1772	1773	rBV	302	191	0.01%	0.002%
45	6.884	1800	1802	1806	rVB2	380	282	0.02%	0.002%
46	6.987	1821	1834	1860	rBV	212909	389420	24.86%	3.068%
47	7.318	1925	1937	1963	rBV	739378	1278821	81.63%	10.073%
48	7.624	2022	2032	2058	rBV	147149	255700	16.32%	2.014%
49	7.804	2086	2088	2090	rVB	723	229	0.01%	0.002%
50	7.843	2097	2100	2101	rBV	687	338	0.02%	0.003%
51	7.984	2141	2144	2145	rBV3	759	474	0.03%	0.004%
52	8.013	2151	2153	2155	rBV	435	185	0.01%	0.001%
53	8.039	2159	2161	2165	rVB2	650	292	0.02%	0.002%
54	8.090	2166	2177	2223	rBV2	390602	796893	50.86%	6.277%
55	8.482	2297	2299	2301	rBV	435	292	0.02%	0.002%
56	8.531	2311	2314	2316	rBV3	357	219	0.01%	0.002%
57	8.601	2333	2336	2341	rVB5	781	669	0.04%	0.005%
58	8.855	2403	2415	2435	rBV	838681	1338673	85.45%	10.545%
59	9.058	2475	2478	2484	rBV4	961	720	0.05%	0.006%
60	9.338	2561	2565	2566	rBV3	798	519	0.03%	0.004%
61	9.495	2612	2614	2619	rBV2	503	393	0.03%	0.003%
62	9.550	2628	2631	2633	rBV	620	395	0.03%	0.003%
63	9.595	2642	2645	2647	rVV	567	287	0.02%	0.002%
64	9.653	2662	2663	2666	rBV	421	200	0.01%	0.002%
65	9.717	2680	2683	2690	rVB4	537	482	0.03%	0.004%
66	9.913	2739	2744	2747	rBV4	484	462	0.03%	0.004%
67	10.035	2781	2782	2786	rVB	401	234	0.01%	0.002%
68	10.138	2811	2814	2815	rBV	724	467	0.03%	0.004%
69	10.222	2828	2840	2858	rVV	466353	732097	46.73%	5.767%
70	10.441	2906	2908	2911	rVB4	532	237	0.02%	0.002%
71	10.460	2911	2914	2916	rVV3	513	240	0.02%	0.002%
72	10.534	2935	2937	2940	rBV3	387	287	0.02%	0.002%
73	10.714	2989	2993	3000	rVB3	870	785	0.05%	0.006%
74	10.749	3000	3004	3007	rBV5	544	477	0.03%	0.004%
75	10.978	3073	3075	3076	rBV	502	233	0.01%	0.002%
76	11.042	3093	3095	3101	rVB4	607	479	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012521\
 Data File : VV020152.D
 Acq On : 25 Jan 2021 10:53
 Operator : SY/MD
 Sample : VV0125WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M

Title : VOC Analysis

77	11.080	3104	3107	3112	rBV2	681	556	0.04%	0.004%
78	11.183	3133	3139	3141	rBV4	986	984	0.06%	0.008%
79	11.254	3150	3161	3181	rBV	789121	1233587	78.74%	9.717%
80	11.495	3232	3236	3237	rBV	537	351	0.02%	0.003%
81	11.630	3266	3278	3298	rBV	762436	1204932	76.91%	9.491%
82	11.772	3319	3322	3324	rBV3	1006	738	0.05%	0.006%
83	12.164	3442	3444	3447	rBV	446	229	0.01%	0.002%
84	12.260	3472	3474	3481	rVB3	678	607	0.04%	0.005%
85	12.302	3481	3487	3494	rBV2	530	716	0.05%	0.006%
86	12.592	3574	3577	3579	rBV2	452	218	0.01%	0.002%
87	12.621	3583	3586	3589	rVB2	353	193	0.01%	0.002%
88	12.659	3589	3598	3599	rBV	973	966	0.06%	0.008%
89	12.733	3617	3621	3624	rVB	294	197	0.01%	0.002%
90	12.910	3671	3676	3682	rBV2	289	337	0.02%	0.003%
91	13.051	3717	3720	3725	rBV2	367	271	0.02%	0.002%
92	13.132	3742	3745	3749	rBV3	331	284	0.02%	0.002%
93	13.276	3785	3790	3795	rBV3	1632	1885	0.12%	0.015%
94	13.325	3801	3805	3810	rBV3	572	642	0.04%	0.005%
95	13.421	3830	3835	3838	rBV2	410	357	0.02%	0.003%
96	13.437	3838	3840	3845	rVV2	239	271	0.02%	0.002%
97	13.518	3862	3865	3866	rBV	1065	654	0.04%	0.005%
98	13.608	3890	3893	3898	rBV2	368	298	0.02%	0.002%
99	13.656	3904	3908	3912	rBV3	372	422	0.03%	0.003%
100	13.759	3936	3940	3950	rVB6	1260	1848	0.12%	0.015%




Sum of corrected areas: 12694957

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012521\
Data File : VV020152.D
Acq On : 25 Jan 2021 10:53
Operator : SY/MD
Sample : VV0125WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

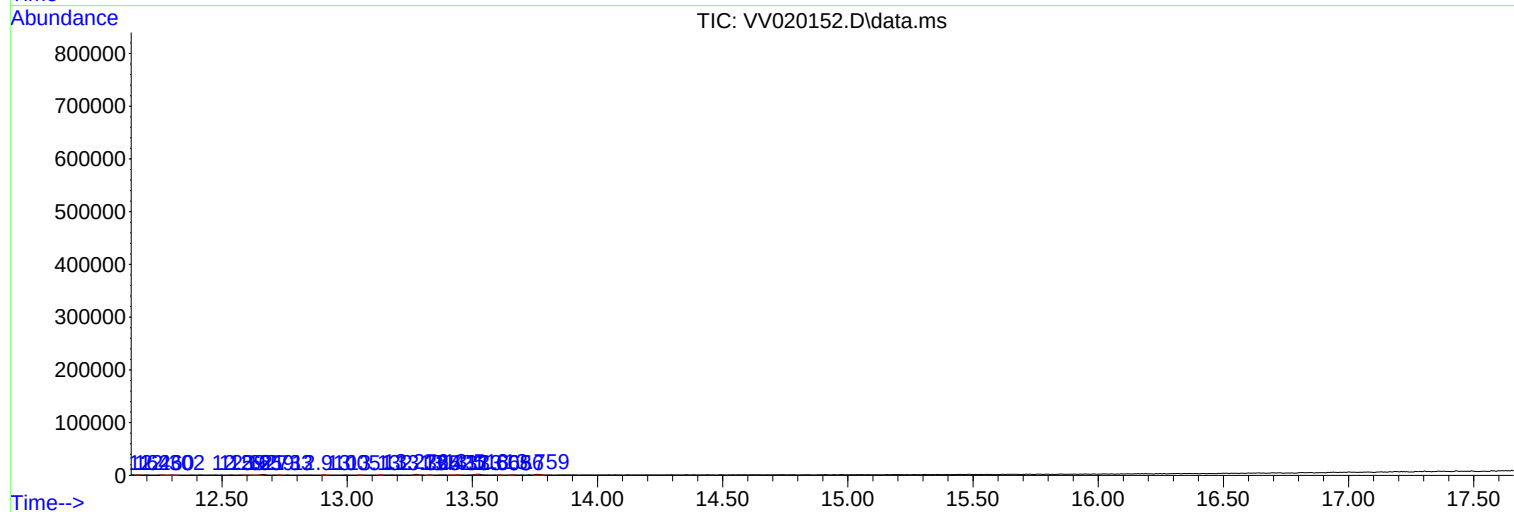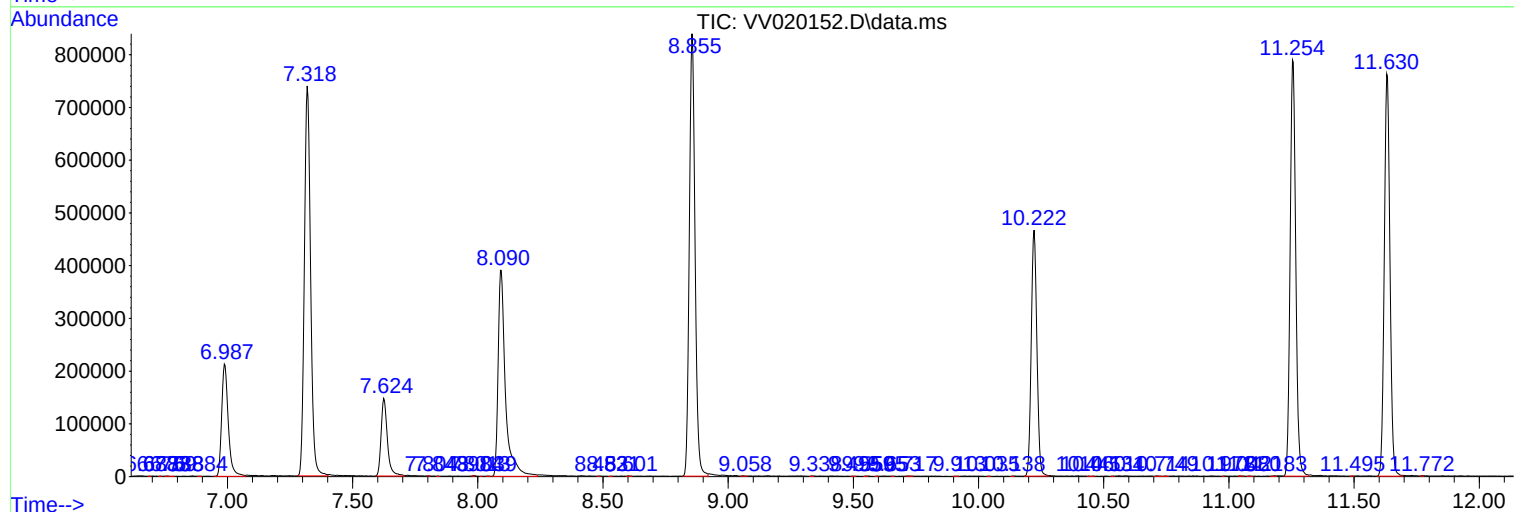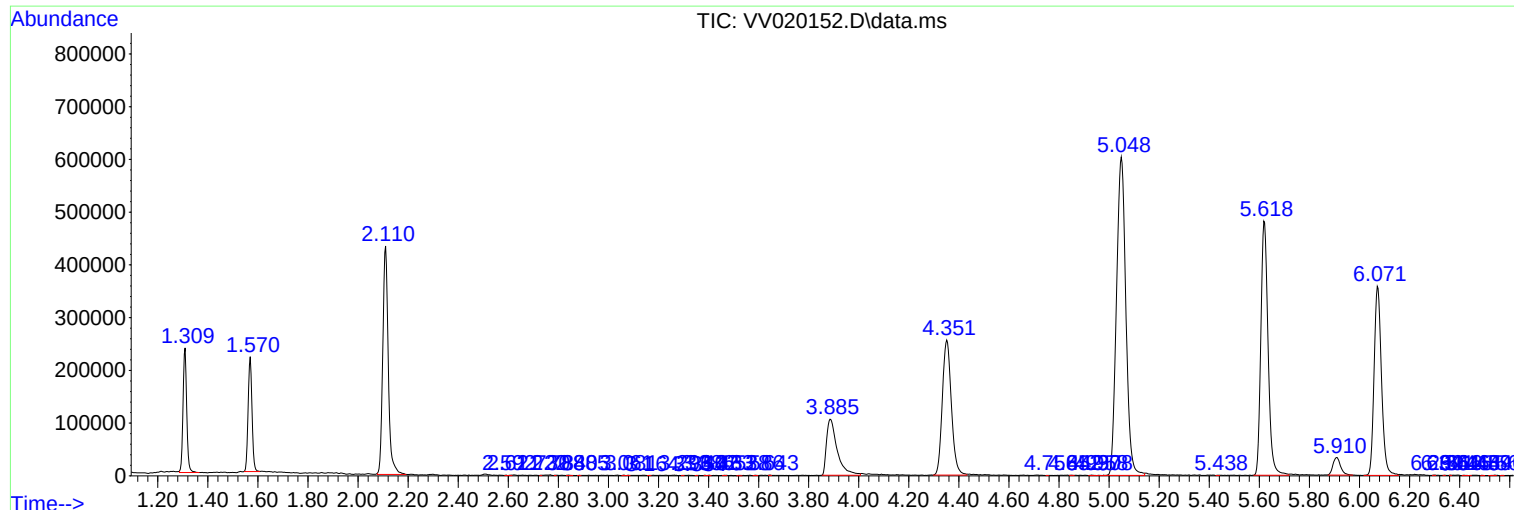

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012521\
Data File : VV020152.D
Acq On : 25 Jan 2021 10:53
Operator : SY/MD
Sample : VV0125WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012521\
Data File : VV020152.D
Acq On : 25 Jan 2021 10:53
Operator : SY/MD
Sample : VV0125WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
