
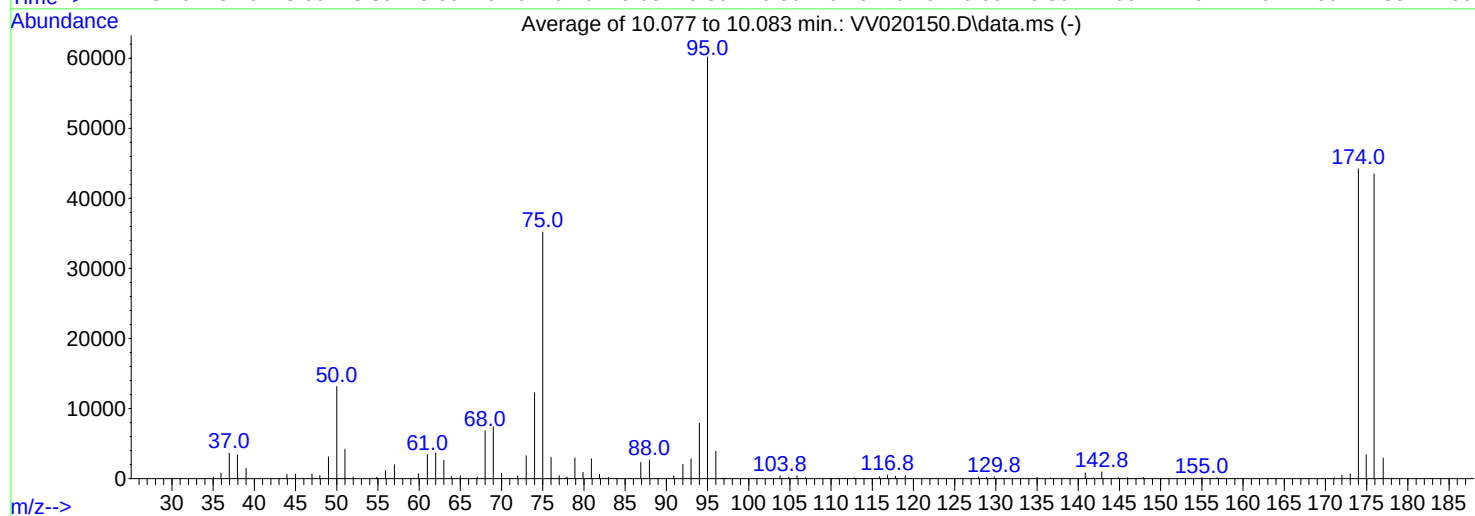


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012521\
 Data File : VV020150.D
 Acq On : 25 Jan 2021 09:00
 Operator : SY/MD
 Sample : BFB87
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB87

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM012121WMA.M
 Title : VOC Analysis
 Last Update : Mon Jan 25 15:30:53 2021

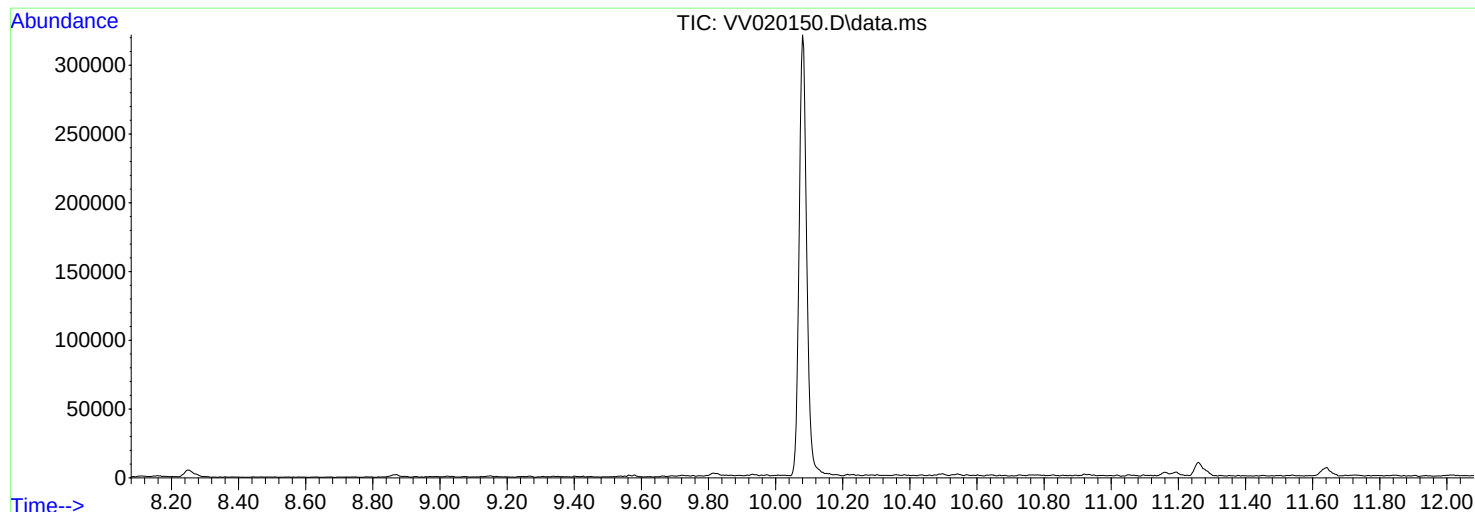

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	13155	PASS
75	95	30	80	58.5	35192	PASS
95	95	100	100	100.0	60203	PASS
96	95	5	9	6.5	3937	PASS
173	174	0.00	2	1.6	692	PASS
174	95	50	120	73.4	44213	PASS
175	174	5	9	7.8	3432	PASS
176	174	95	101	98.4	43509	PASS
177	176	5	9	6.8	2938	PASS

m/z	Abundance
36.00	611.0
36.90	122.0
37.90	228.0
39.90	252.0
41.80	116.0
44.10	303.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.00	228.0
35.90	1570.0
37.00	3547.0
38.00	3513.0
39.00	1439.0
39.80	246.0
41.00	110.0
44.00	956.0
45.00	627.0
47.00	758.0
47.90	459.0
49.00	2876.0
50.00	12823.0
51.00	4163.0
52.00	291.0
54.80	229.0
55.90	1193.0
57.00	1806.0
57.90	114.0
59.00	107.0
59.90	777.0
61.00	3292.0
62.00	3696.0
63.00	2451.0
63.90	278.0
65.00	454.0
67.10	216.0
68.00	7006.0
69.00	7183.0
70.00	788.0
71.90	386.0
73.00	2899.0
74.00	11816.0
75.00	34944.0
76.00	3038.0
77.00	440.0
77.80	271.0
78.00	262.0
78.90	2852.0
79.90	851.0
80.90	2826.0
81.90	550.0
83.00	199.0
85.70	144.0
86.90	2241.0
88.00	2581.0
90.90	401.0
92.00	1995.0
93.00	2641.0
94.00	7948.0
95.00	57824.0
96.00	3720.0
96.80	164.0
103.80	392.0
104.90	216.0
105.80	350.0
106.80	135.0
112.80	117.0
115.80	284.0
116.90	514.0
117.80	408.0
119.00	452.0
127.90	238.0
128.80	185.0
129.80	228.0
130.90	114.0
135.00	193.0
136.60	101.0
140.90	778.0
141.80	140.0
142.80	1002.0
144.90	158.0
146.00	138.0
147.90	184.0
152.80	116.0
155.00	148.0
156.80	133.0
172.00	448.0
173.00	606.0
174.00	41568.0
174.90	3070.0
175.90	40424.0
177.00	2728.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.10	235.0
35.90	1426.0
37.00	3914.0
38.00	3762.0
39.00	1511.0
39.80	287.0
40.90	113.0
43.90	970.0
45.00	695.0
45.90	125.0
47.00	693.0
47.90	486.0
49.00	3225.0
50.00	13601.0
51.00	4365.0
52.00	255.0
54.80	208.0
55.90	1178.0
57.00	2066.0
57.90	112.0
59.90	709.0
61.00	3580.0
62.00	3838.0
63.00	2698.0
63.90	301.0
65.00	452.0
67.00	240.0
68.00	7008.0
69.00	7703.0
70.00	803.0
71.90	356.0
73.00	3362.0
74.00	12719.0
75.00	36432.0
76.00	3147.0
77.00	454.0
77.90	254.0
78.90	3017.0
79.90	947.0
80.90	2934.0
81.90	633.0
82.90	196.0
86.90	2353.0
88.00	2735.0
90.90	419.0
92.00	2079.0
93.00	2903.0
94.00	8133.0
95.00	62224.0
96.00	4047.0
97.20	135.0
103.80	454.0
104.90	207.0
105.90	417.0
106.90	130.0
111.80	139.0
112.80	123.0
115.90	313.0
116.80	538.0
117.80	369.0
119.00	476.0
127.90	257.0
128.80	197.0
129.80	275.0
135.00	200.0
136.70	148.0
140.90	840.0
141.90	142.0
142.90	1003.0
144.90	144.0
146.00	145.0
147.90	174.0
155.00	169.0
156.80	142.0
169.50	104.0
171.10	144.0
172.00	492.0
173.00	722.0
174.00	45664.0
175.00	3520.0
175.90	45104.0
177.00	3036.0
178.00	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.10	210.0
36.00	1253.0
37.00	3825.0
38.00	3637.0
39.00	1442.0
39.80	280.0
43.90	857.0
45.00	641.0
45.90	136.0
47.00	547.0
48.00	455.0
49.00	3198.0
50.00	13042.0
51.00	4058.0
52.00	218.0
54.90	196.0
55.90	1123.0
57.00	2075.0
59.90	665.0
61.00	3504.0
62.00	3513.0
63.00	2754.0
63.90	336.0
65.00	397.0
67.00	245.0
68.00	6449.0
69.00	7403.0
70.00	707.0
70.90	123.0
72.00	331.0
73.00	3565.0
74.00	12247.0
75.00	34200.0
76.00	2962.0
77.00	406.0
77.90	202.0
78.90	2971.0
79.90	931.0
80.90	2765.0
81.90	691.0
82.90	153.0
86.90	2352.0
87.90	2613.0
90.90	400.0
92.00	2013.0
93.00	2981.0
94.00	7667.0
95.00	60560.0
96.00	4044.0
97.20	101.0
103.80	418.0
104.80	178.0
105.90	448.0
107.00	132.0
110.80	109.0
111.80	151.0
112.80	110.0
115.90	324.0
116.80	528.0
117.80	295.0
119.00	403.0
127.90	261.0
128.90	171.0
129.80	301.0
135.00	158.0
136.70	196.0
140.80	878.0
142.00	120.0
142.90	892.0
144.80	122.0
146.00	121.0
147.90	134.0
155.00	168.0
156.90	150.0
158.90	131.0
171.10	177.0
172.00	500.0
173.00	747.0
174.00	45408.0
175.00	3707.0
175.90	45000.0
177.00	3049.0
178.00	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87