

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
 Data File : VV029936.D
 Acq On : 25 Jan 2023 12:14
 Operator : SY/MD
 Sample : VV0125WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK297

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029936.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	87720	88541	15.81%	1.753%
2	1.565	155	163	178	rVB	86931	97279	17.37%	1.926%
3	2.101	320	330	347	rBV	140243	205182	36.63%	4.061%
4	2.500	444	454	470	rVB2	16203	27023	4.82%	0.535%
5	3.892	874	887	935	rBV2	62573	241653	43.14%	4.783%
6	4.336	1007	1025	1047	rBV	104666	261311	46.65%	5.172%
7	5.037	1226	1243	1270	rBV2	221242	560200	100.00%	11.088%
8	5.606	1408	1420	1453	rBV	180635	384729	68.68%	7.615%
9	6.060	1548	1561	1590	rBV2	136785	289945	51.76%	5.739%
10	6.979	1836	1847	1860	rBV2	52205	97950	17.48%	1.939%
11	7.307	1935	1949	1973	rBV	233952	417223	74.48%	8.258%
12	7.616	2035	2045	2073	rVB2	30705	57528	10.27%	1.139%
13	7.934	2130	2144	2164	rBV3	17610	37303	6.66%	0.738%
14	8.085	2180	2191	2221	rBV	282060	555055	99.08%	10.987%
15	8.841	2415	2426	2449	rBV	291902	484777	86.54%	9.596%
16	10.204	2840	2850	2873	rVB	111891	177095	31.61%	3.505%
17	10.371	2890	2902	2919	rBV2	38696	65438	11.68%	1.295%
18	11.236	3160	3171	3194	rBV	341847	535130	95.52%	10.592%
19	11.612	3276	3288	3304	rBV	254743	403766	72.08%	7.992%
20	12.239	3471	3483	3495	rVB2	25735	42448	7.58%	0.840%
21	14.027	4030	4039	4049	rVB2	13876	22552	4.03%	0.446%




Sum of corrected areas: 5052128

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029936.D
Acq On : 25 Jan 2023 12:14
Operator : SY/MD
Sample : VV0125WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK297

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

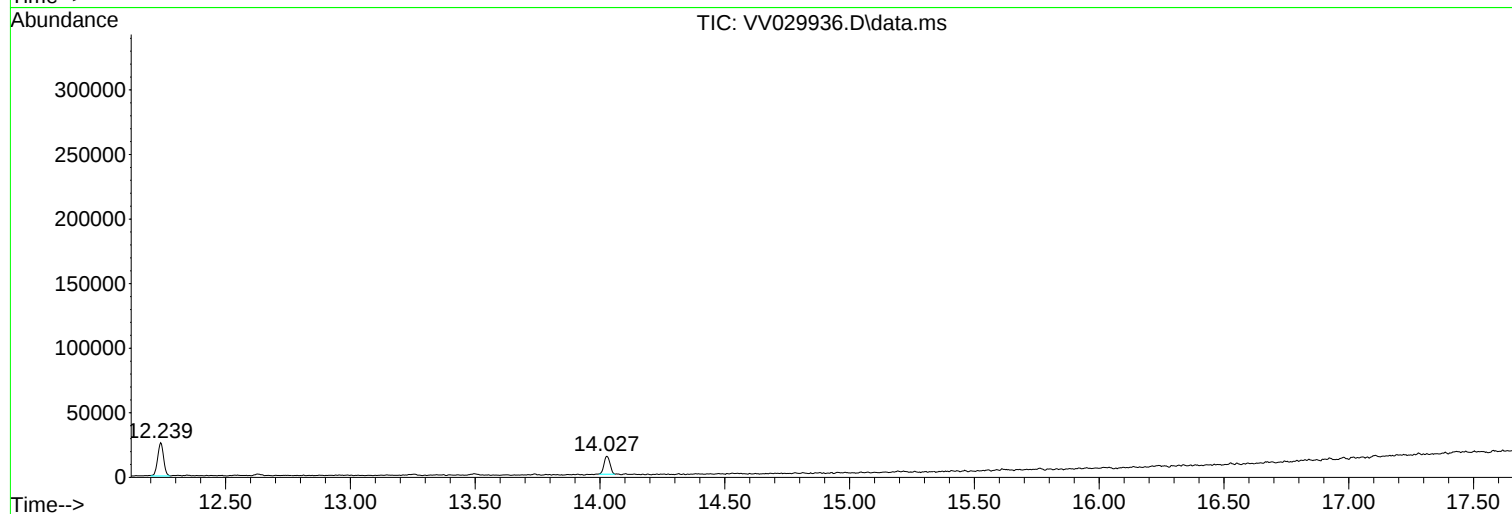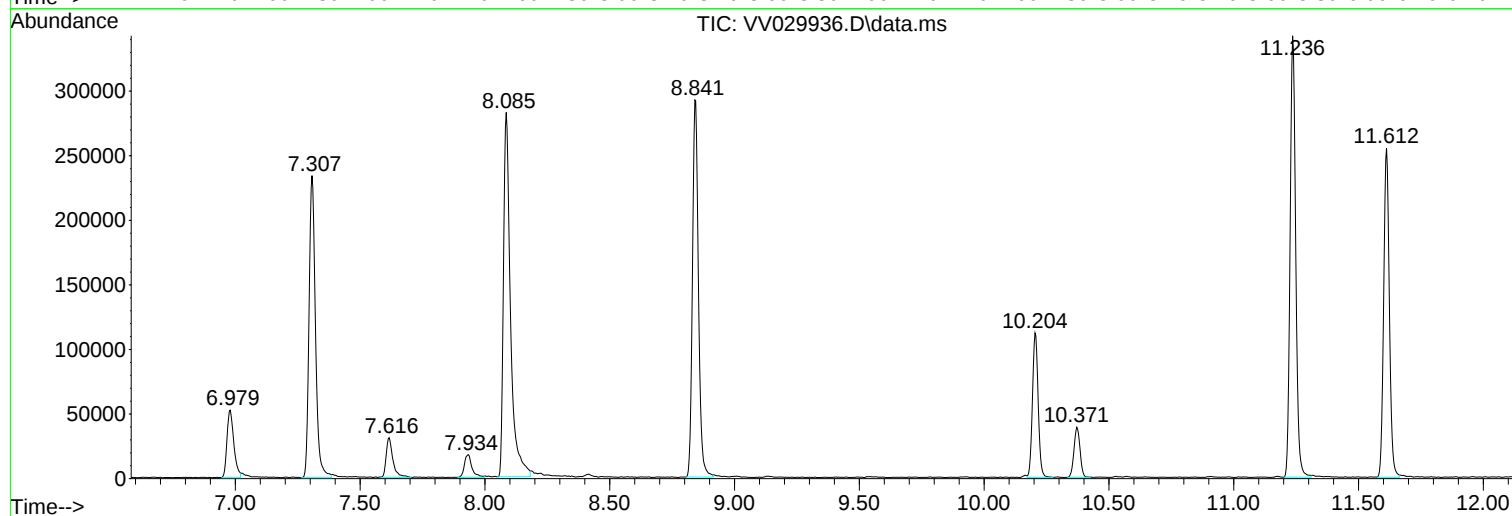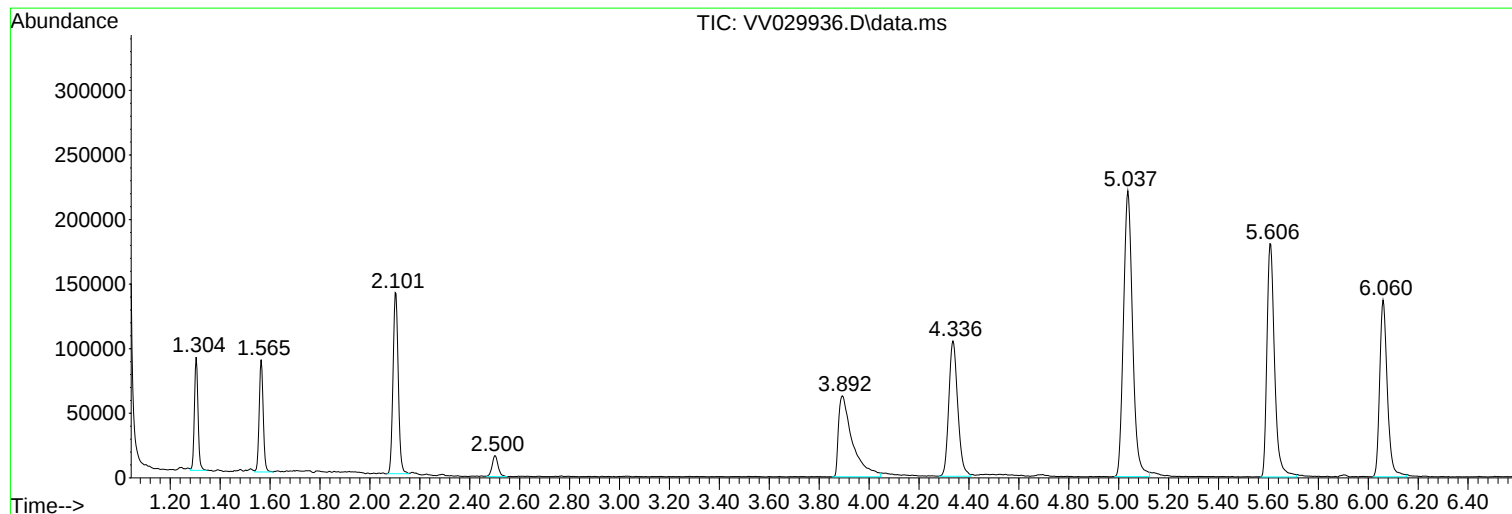

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029936.D
Acq On : 25 Jan 2023 12:14
Operator : SY/MD
Sample : VV0125WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK297

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029936.D
Acq On : 25 Jan 2023 12:14
Operator : SY/MD
Sample : VV0125WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK297

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc