

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
 Data File : VV029938.D
 Acq On : 25 Jan 2023 13:03
 Operator : SY/MD
 Sample : 01277-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9G7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	87538	90468	15.52%	1.812%
2	1.568	156	164	175	rVB	86837	97724	16.77%	1.958%
3	2.104	321	331	349	rVB	144150	211281	36.25%	4.232%
4	2.503	442	455	465	rBV3	5667	8709	1.49%	0.174%
5	3.889	872	886	929	rBV	73543	251770	43.20%	5.043%
6	4.339	1009	1026	1055	rBV	109507	281227	48.25%	5.634%
7	5.040	1227	1244	1274	rBV2	226817	578547	99.26%	11.589%
8	5.609	1408	1421	1442	rBV	173969	356790	61.22%	7.147%
9	6.063	1548	1562	1602	rBV	142764	301378	51.71%	6.037%
10	6.979	1834	1847	1868	rBV2	52698	103453	17.75%	2.072%
11	7.310	1937	1950	1970	rBV	237126	425338	72.98%	8.520%
12	7.616	2036	2045	2067	rBV	31633	59488	10.21%	1.192%
13	7.934	2132	2144	2161	rBV2	16344	32234	5.53%	0.646%
14	8.085	2180	2191	2225	rBV	296104	582837	100.00%	11.675%
15	8.844	2416	2427	2448	rBV	271457	458991	78.75%	9.195%
16	10.204	2840	2850	2870	rVB	112568	180123	30.90%	3.608%
17	10.371	2888	2902	2915	rBV2	29755	49398	8.48%	0.990%
18	11.236	3160	3171	3194	rBV	308307	489065	83.91%	9.797%
19	11.612	3277	3288	3312	rVB	252549	405662	69.60%	8.126%
20	12.242	3474	3484	3494	rVB2	6842	10805	1.85%	0.216%
21	14.030	4027	4040	4051	rBV	9200	16711	2.87%	0.335%


Sum of corrected areas: 4991999

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029938.D
Acq On : 25 Jan 2023 13:03
Operator : SY/MD
Sample : 01277-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9G7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

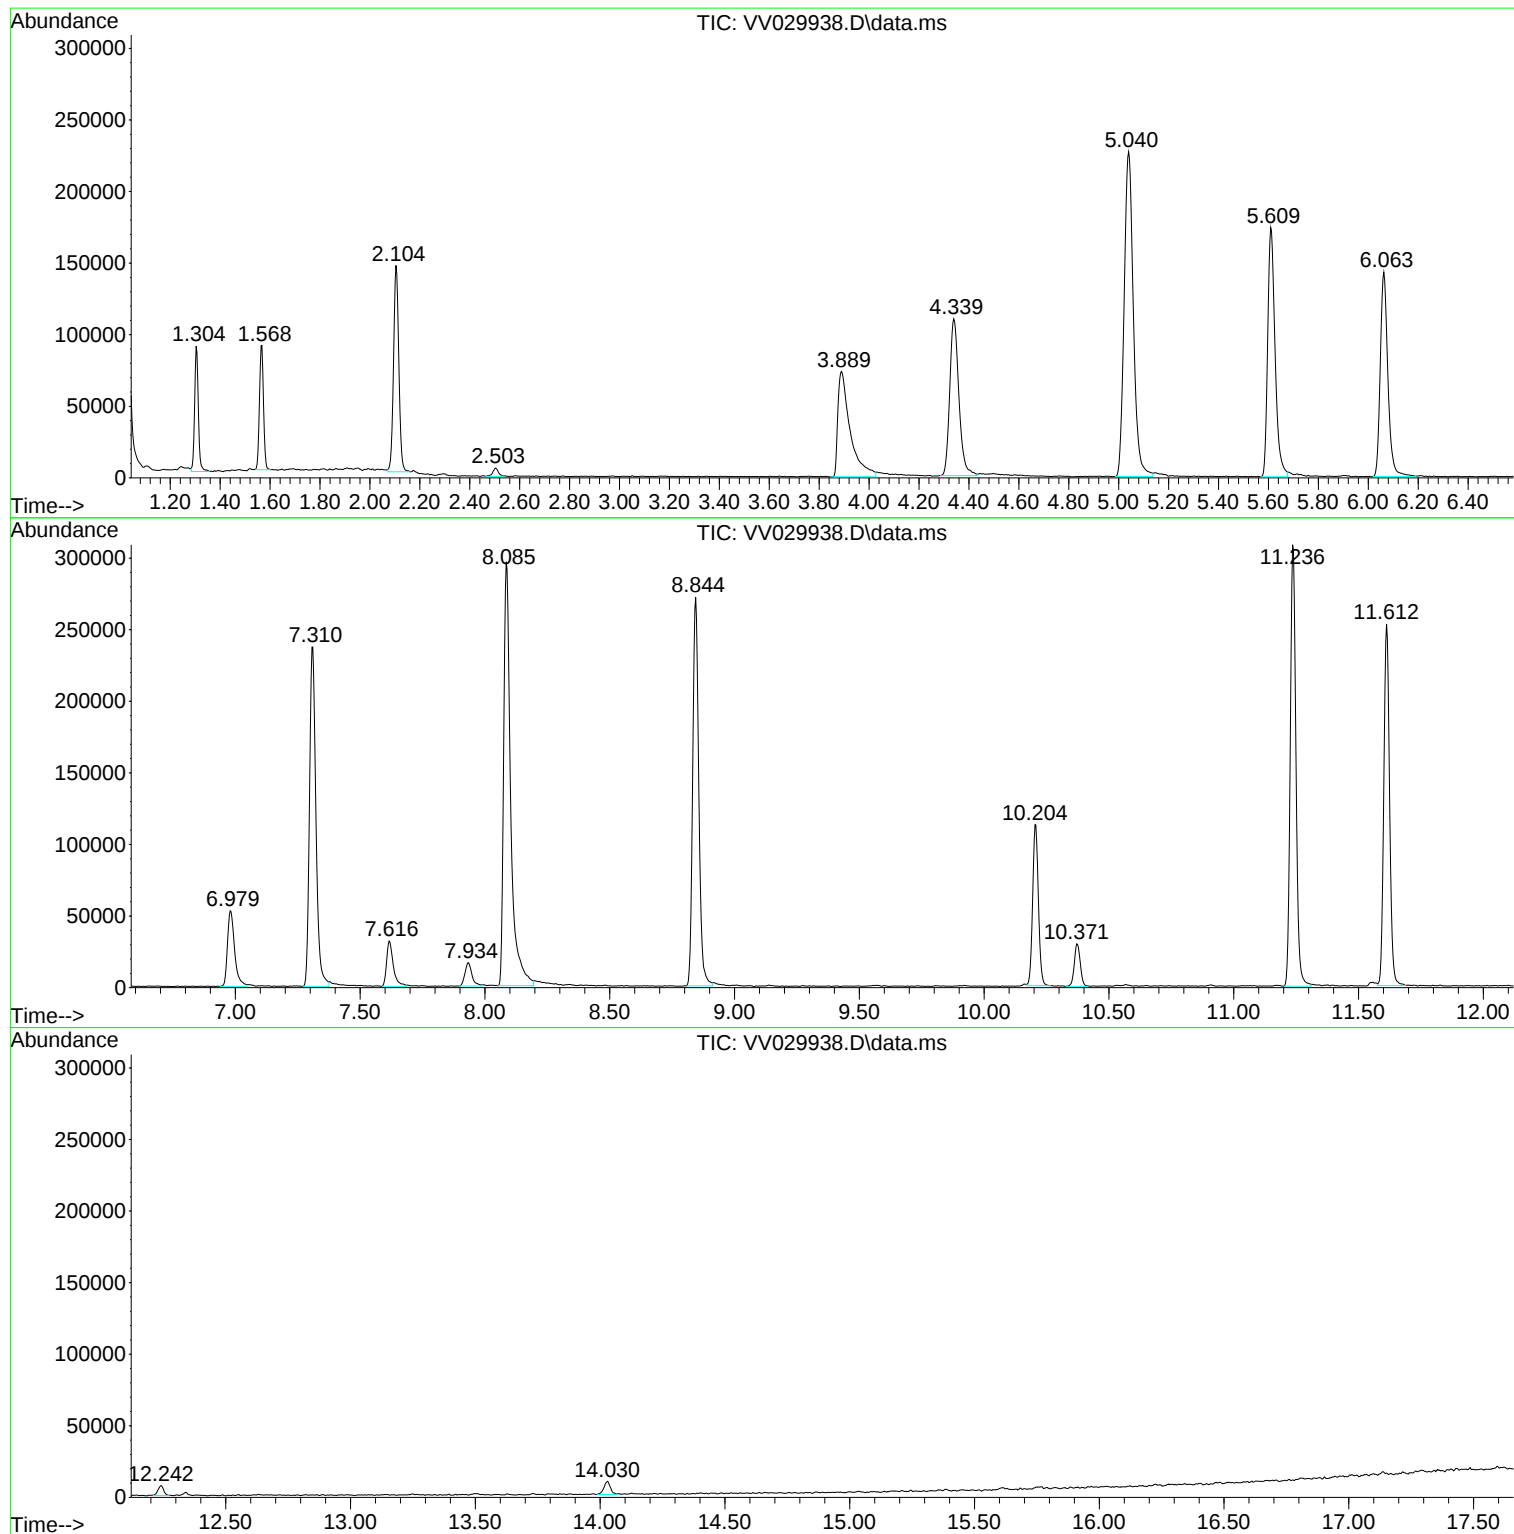

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029938.D
Acq On : 25 Jan 2023 13:03
Operator : SY/MD
Sample : 01277-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9G7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029938.D
Acq On : 25 Jan 2023 13:03
Operator : SY/MD
Sample : 01277-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9G7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------