

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
 Data File : VV029942.D
 Acq On : 25 Jan 2023 14:38
 Operator : SY/MD
 Sample : 01292-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0L58

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	92440	93057	14.62%	1.758%
2	1.565	155	163	175	rVB	95015	105916	16.64%	2.001%
3	2.105	320	331	346	rBV	152335	216983	34.09%	4.100%
4	3.889	876	886	926	rBV	75698	263105	41.33%	4.971%
5	4.339	1010	1026	1053	rBV	112138	285524	44.85%	5.395%
6	5.040	1226	1244	1270	rBV3	237310	613077	96.31%	11.584%
7	5.609	1408	1421	1450	rBV	181900	377817	59.35%	7.139%
8	6.063	1549	1562	1593	rBV	148091	317877	49.93%	6.006%
9	6.979	1837	1847	1865	rBV	57677	108272	17.01%	2.046%
10	7.307	1937	1949	1989	rBV	254162	459442	72.17%	8.681%
11	7.616	2036	2045	2067	rBV2	33043	61252	9.62%	1.157%
12	7.934	2130	2144	2156	rBV3	11946	25131	3.95%	0.475%
13	8.085	2180	2191	2227	rBV	316597	636587	100.00%	12.028%
14	8.844	2415	2427	2458	rBV	287639	486746	76.46%	9.197%
15	10.204	2840	2850	2868	rVB	121985	194707	30.59%	3.679%
16	10.371	2888	2902	2915	rBV	22053	36944	5.80%	0.698%
17	11.236	3160	3171	3192	rBV	338370	534377	83.94%	10.097%
18	11.612	3276	3288	3303	rBV	273310	439900	69.10%	8.312%
19	12.239	3473	3483	3495	rVB	6922	10893	1.71%	0.206%
20	12.336	3507	3513	3523	rBV8	5250	7359	1.16%	0.139%
21	14.027	4029	4039	4050	rVB	10976	17556	2.76%	0.332%




Sum of corrected areas: 5292522

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029942.D
Acq On : 25 Jan 2023 14:38
Operator : SY/MD
Sample : 01292-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

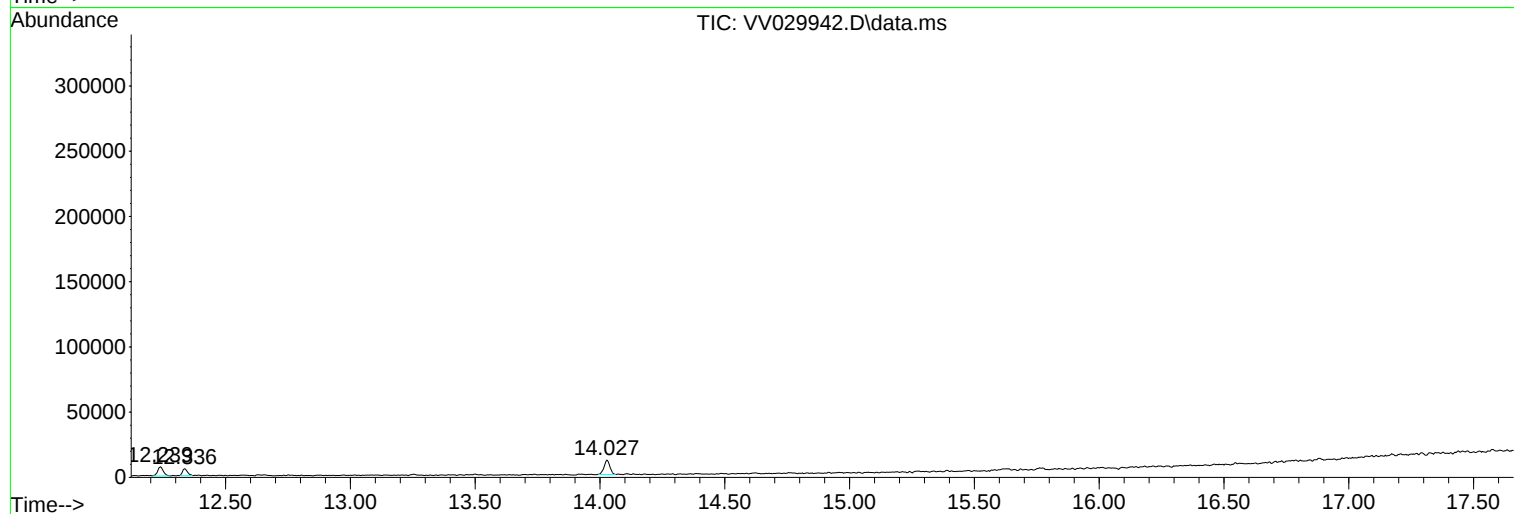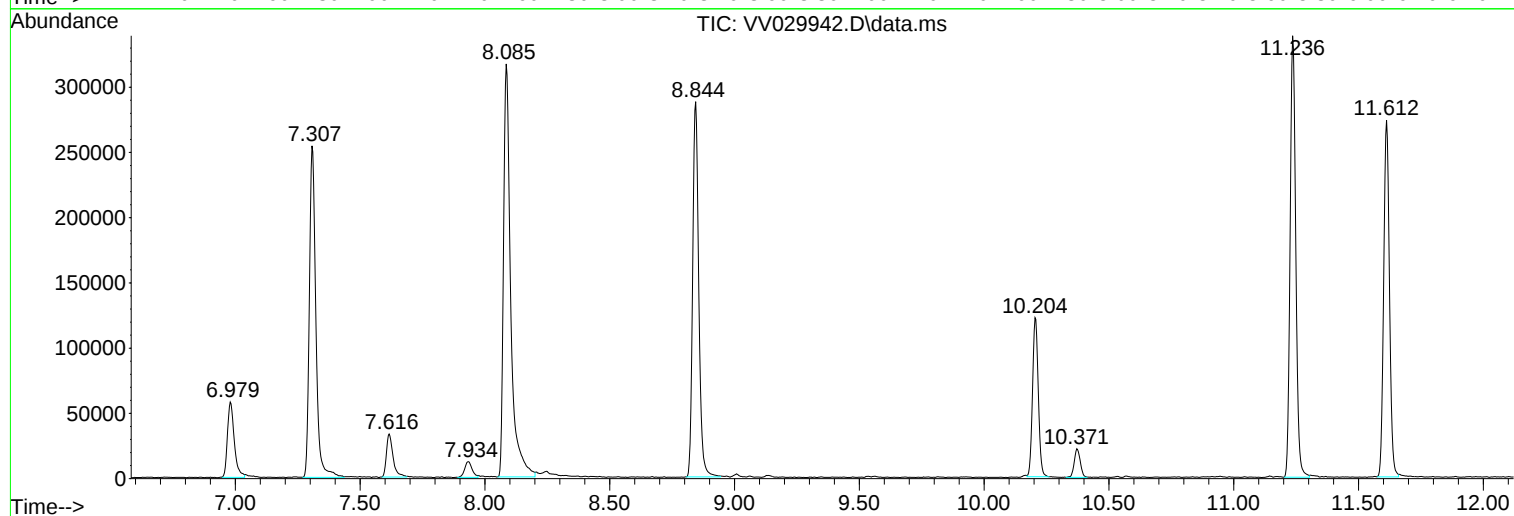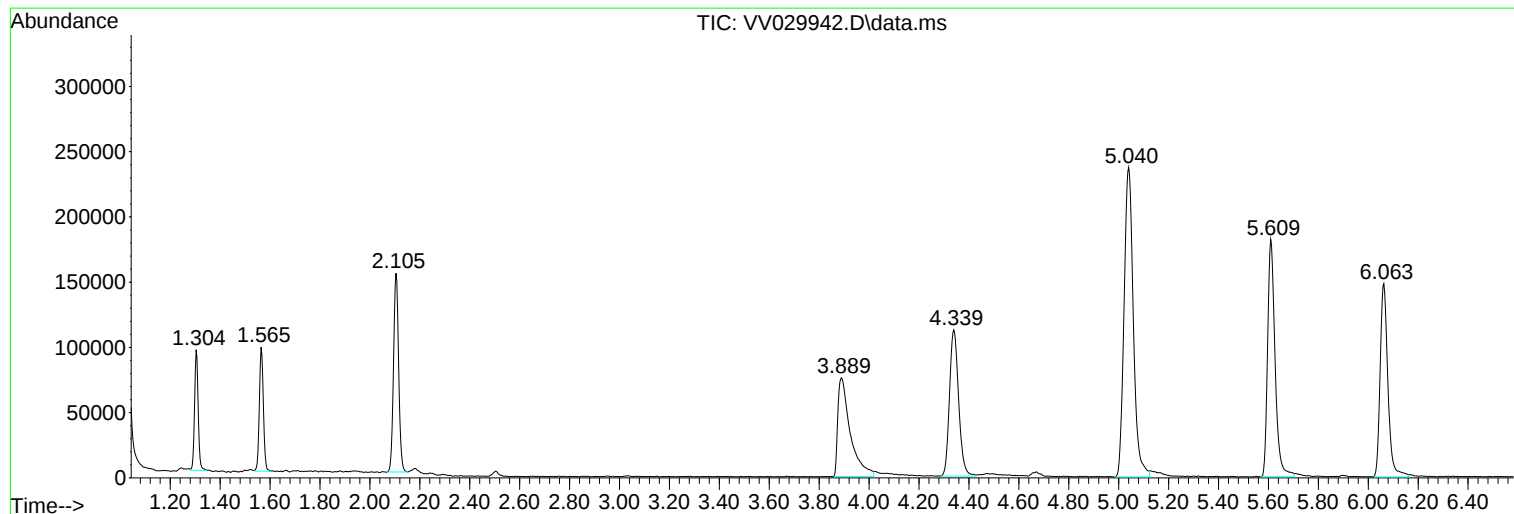

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029942.D
Acq On : 25 Jan 2023 14:38
Operator : SY/MD
Sample : 01292-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029942.D
Acq On : 25 Jan 2023 14:38
Operator : SY/MD
Sample : 01292-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc