

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
 Data File : VV029948.D
 Acq On : 25 Jan 2023 17:29
 Operator : SY/MD
 Sample : 01292-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0L62

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	96	rVB	165439	168091	19.32%	2.239%
2	1.564	155	163	178	rVB	146941	163201	18.76%	2.174%
3	2.104	321	331	347	rVB	253062	362109	41.62%	4.824%
4	2.764	522	536	553	rBV2	16445	36777	4.23%	0.490%
5	3.886	875	885	920	rBV	86088	285052	32.76%	3.798%
6	4.339	1008	1026	1057	rBV	149049	374110	42.99%	4.984%
7	5.040	1227	1244	1275	rBV2	342738	870125	100.00%	11.592%
8	5.609	1407	1421	1446	rBV	257613	537295	61.75%	7.158%
9	5.908	1501	1514	1538	rBV	138287	281659	32.37%	3.752%
10	6.063	1548	1562	1584	rBV	196563	411968	47.35%	5.489%
11	6.979	1835	1847	1873	rBV2	80859	154706	17.78%	2.061%
12	7.307	1937	1949	1964	rBV	404256	707985	81.37%	9.432%
13	7.381	1964	1972	1990	rVB	51674	98680	11.34%	1.315%
14	7.616	2031	2045	2071	rBV	46558	87732	10.08%	1.169%
15	7.931	2131	2143	2162	rBV2	12564	26005	2.99%	0.346%
16	8.085	2180	2191	2235	rBV	355021	696699	80.07%	9.282%
17	8.844	2414	2427	2451	rBV	394741	660405	75.90%	8.798%
18	10.204	2840	2850	2868	rVB	137657	217911	25.04%	2.903%
19	10.374	2892	2903	2913	rVB	32038	53677	6.17%	0.715%
20	11.236	3160	3171	3193	rBV	410724	642057	73.79%	8.554%
21	11.612	3277	3288	3313	rBV	372200	590807	67.90%	7.871%
22	12.239	3473	3483	3499	rVB2	14890	24166	2.78%	0.322%
23	12.339	3505	3514	3524	rBV4	5781	8817	1.01%	0.117%
24	13.249	3789	3797	3810	rBV2	7279	9860	1.13%	0.131%
25	13.493	3861	3873	3885	rBV	14099	23324	2.68%	0.311%
26	13.731	3939	3947	3960	rVB3	7793	12800	1.47%	0.171%




Sum of corrected areas: 7506018

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029948.D
Acq On : 25 Jan 2023 17:29
Operator : SY/MD
Sample : 01292-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

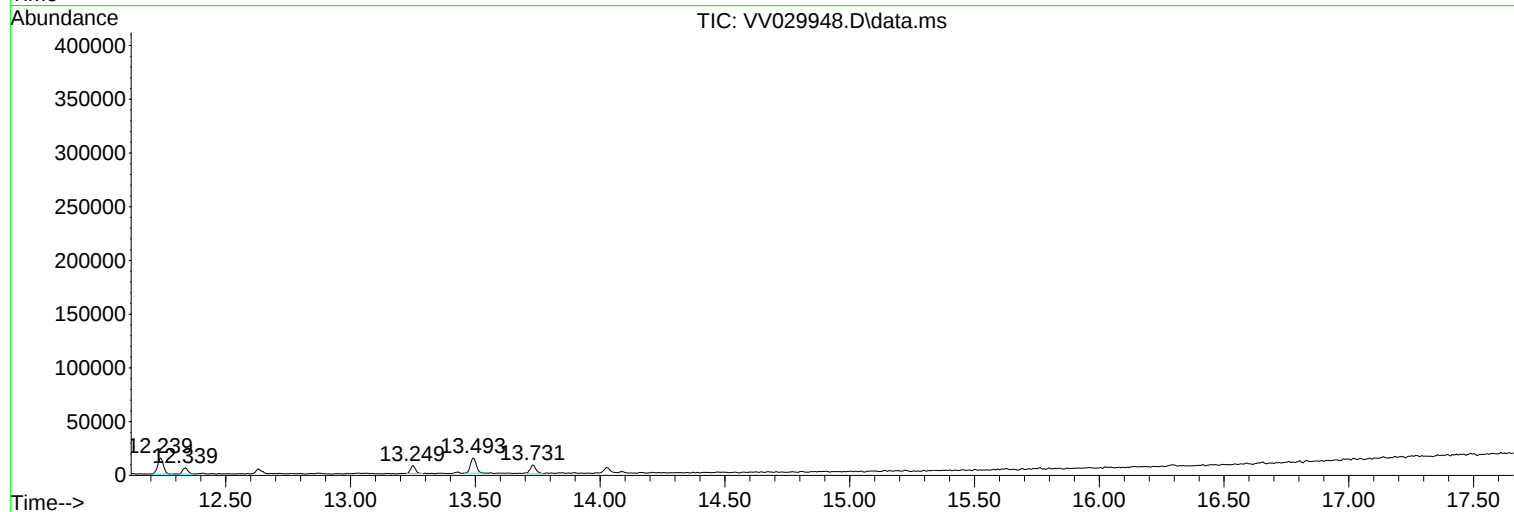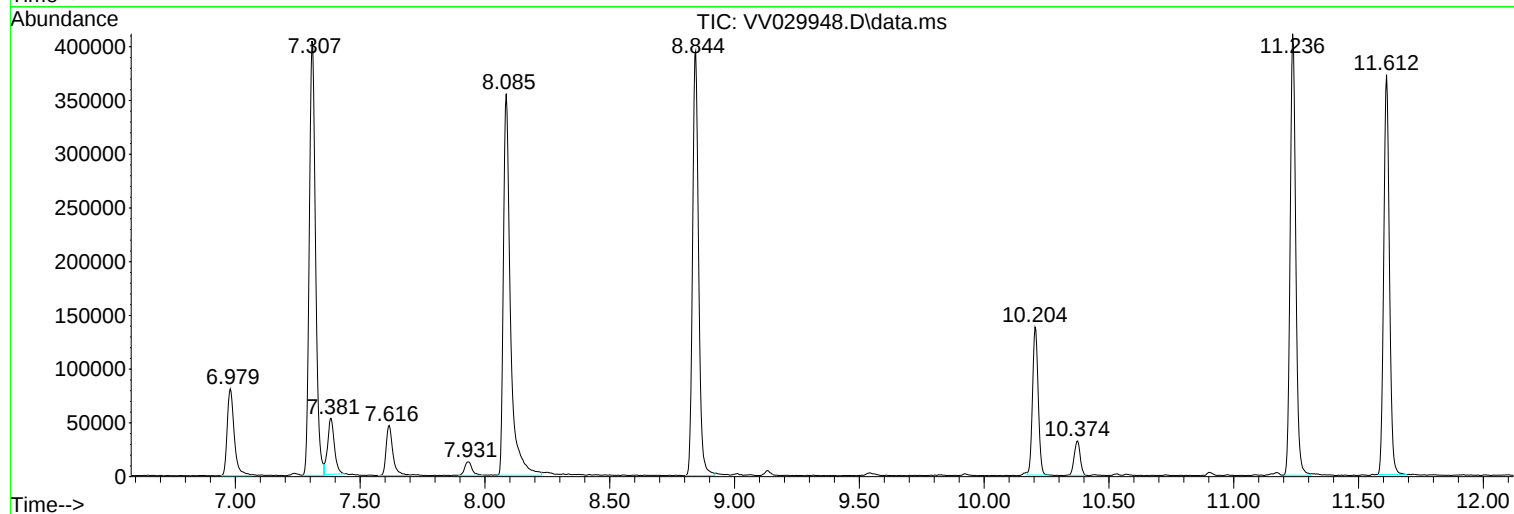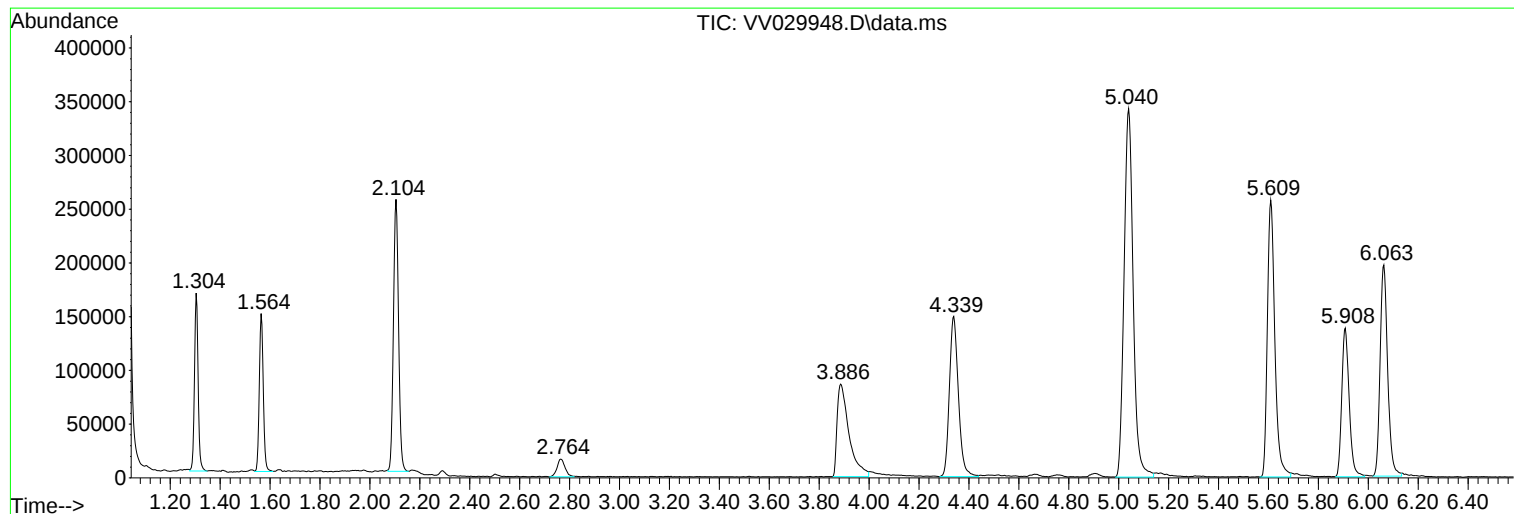

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029948.D
Acq On : 25 Jan 2023 17:29
Operator : SY/MD
Sample : 01292-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029948.D
Acq On : 25 Jan 2023 17:29
Operator : SY/MD
Sample : 01292-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
