

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
 Data File : VV029955.D
 Acq On : 25 Jan 2023 20:15
 Operator : SY/MD
 Sample : 01292-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0L69

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029955.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	100	rVB	159784	170579	20.33%	2.435%
2	1.564	155	163	183	rVB	142972	159256	18.98%	2.273%
3	2.105	320	331	348	rBV	247803	356243	42.45%	5.085%
4	3.886	874	885	922	rBV	81247	258925	30.85%	3.696%
5	4.339	1008	1026	1057	rBV	144652	362184	43.16%	5.170%
6	5.040	1226	1244	1270	rBV2	331083	839206	100.00%	11.979%
7	5.609	1408	1421	1446	rBV	263496	547846	65.28%	7.820%
8	5.912	1502	1515	1540	rBV4	11141	24480	2.92%	0.349%
9	6.063	1546	1562	1590	rBV	197728	411722	49.06%	5.877%
10	6.979	1837	1847	1871	rBV	78082	146201	17.42%	2.087%
11	7.307	1937	1949	1966	rBV	385885	685392	81.67%	9.783%
12	7.384	1967	1973	1986	rVB	12929	25279	3.01%	0.361%
13	7.616	2032	2045	2072	rBV	44941	84475	10.07%	1.206%
14	7.934	2130	2144	2152	rBV3	6355	11993	1.43%	0.171%
15	8.085	2180	2191	2223	rBV	353853	680119	81.04%	9.708%
16	8.844	2415	2427	2450	rBV	417335	678747	80.88%	9.688%
17	9.776	2709	2717	2728	rBV4	5843	10747	1.28%	0.153%
18	10.204	2840	2850	2872	rVB	139750	220159	26.23%	3.143%
19	10.371	2891	2902	2914	rVB2	13827	22305	2.66%	0.318%
20	10.616	2968	2978	2993	rBV4	5910	11898	1.42%	0.170%
21	11.085	3113	3124	3136	rBV3	7343	11397	1.36%	0.163%
22	11.201	3149	3160	3162	rBV	24504	30845	3.68%	0.440%
23	11.236	3162	3171	3197	rVB	425501	667037	79.48%	9.521%
24	11.612	3276	3288	3305	rBV	364608	578189	68.90%	8.253%
25	12.239	3469	3483	3495	rBV2	5991	10549	1.26%	0.151%




Sum of corrected areas: 7005773

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029955.D
Acq On : 25 Jan 2023 20:15
Operator : SY/MD
Sample : 01292-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL69

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

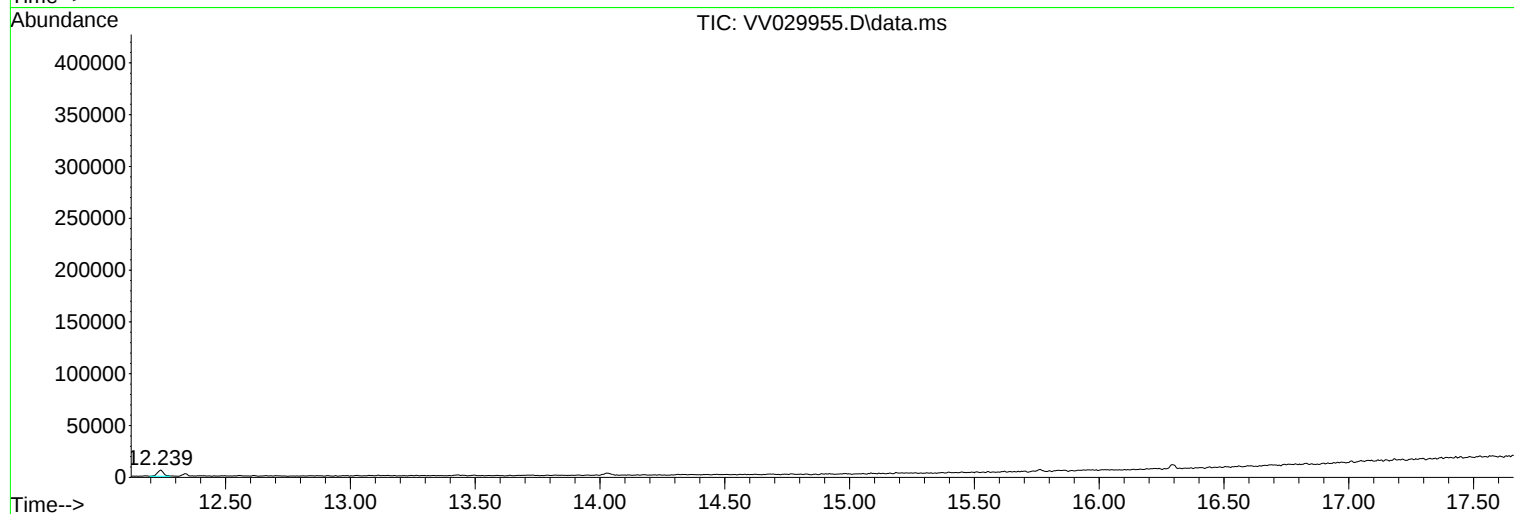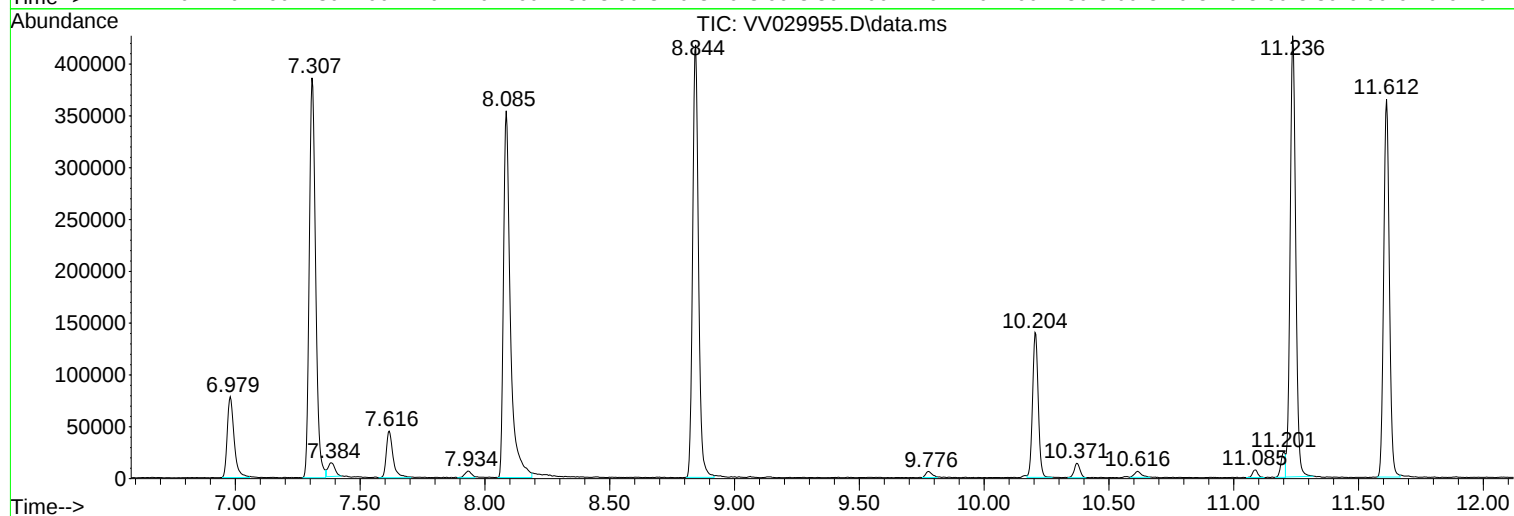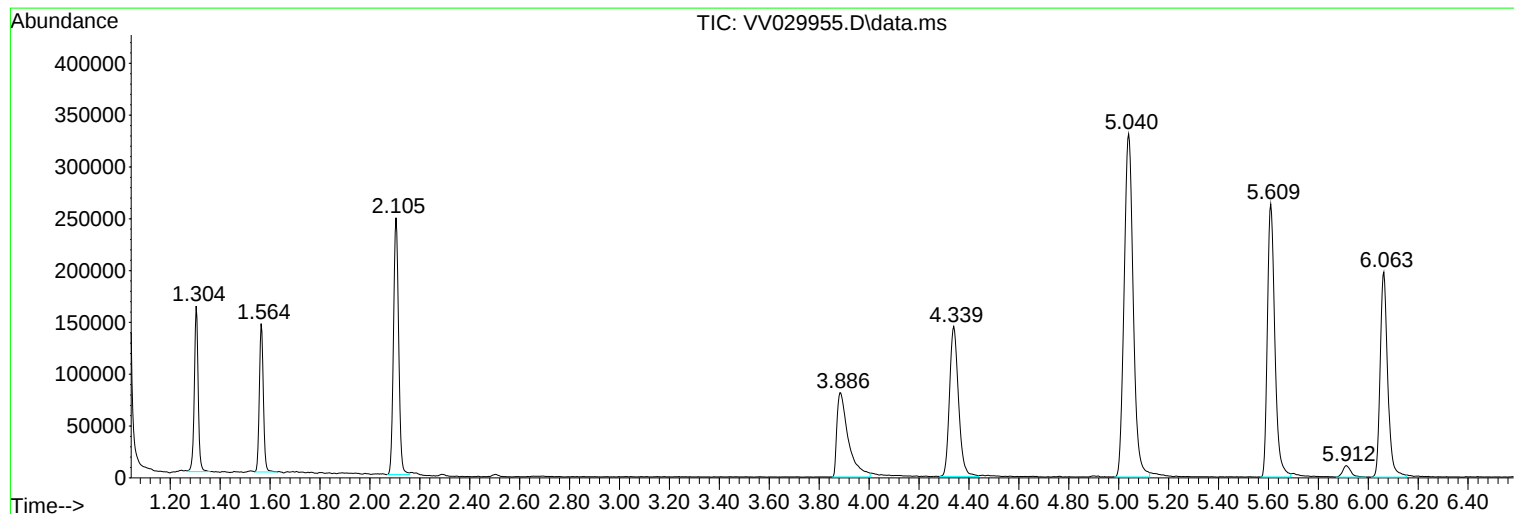

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029955.D
Acq On : 25 Jan 2023 20:15
Operator : SY/MD
Sample : 01292-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L69

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029955.D
Acq On : 25 Jan 2023 20:15
Operator : SY/MD
Sample : 01292-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L69

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc