


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012523\
Data File : VV029934.D
Acq On : 25 Jan 2023 09:39
Operator : SY/MD
Sample : BFB216
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB216

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jan 27 01:28:41 2023

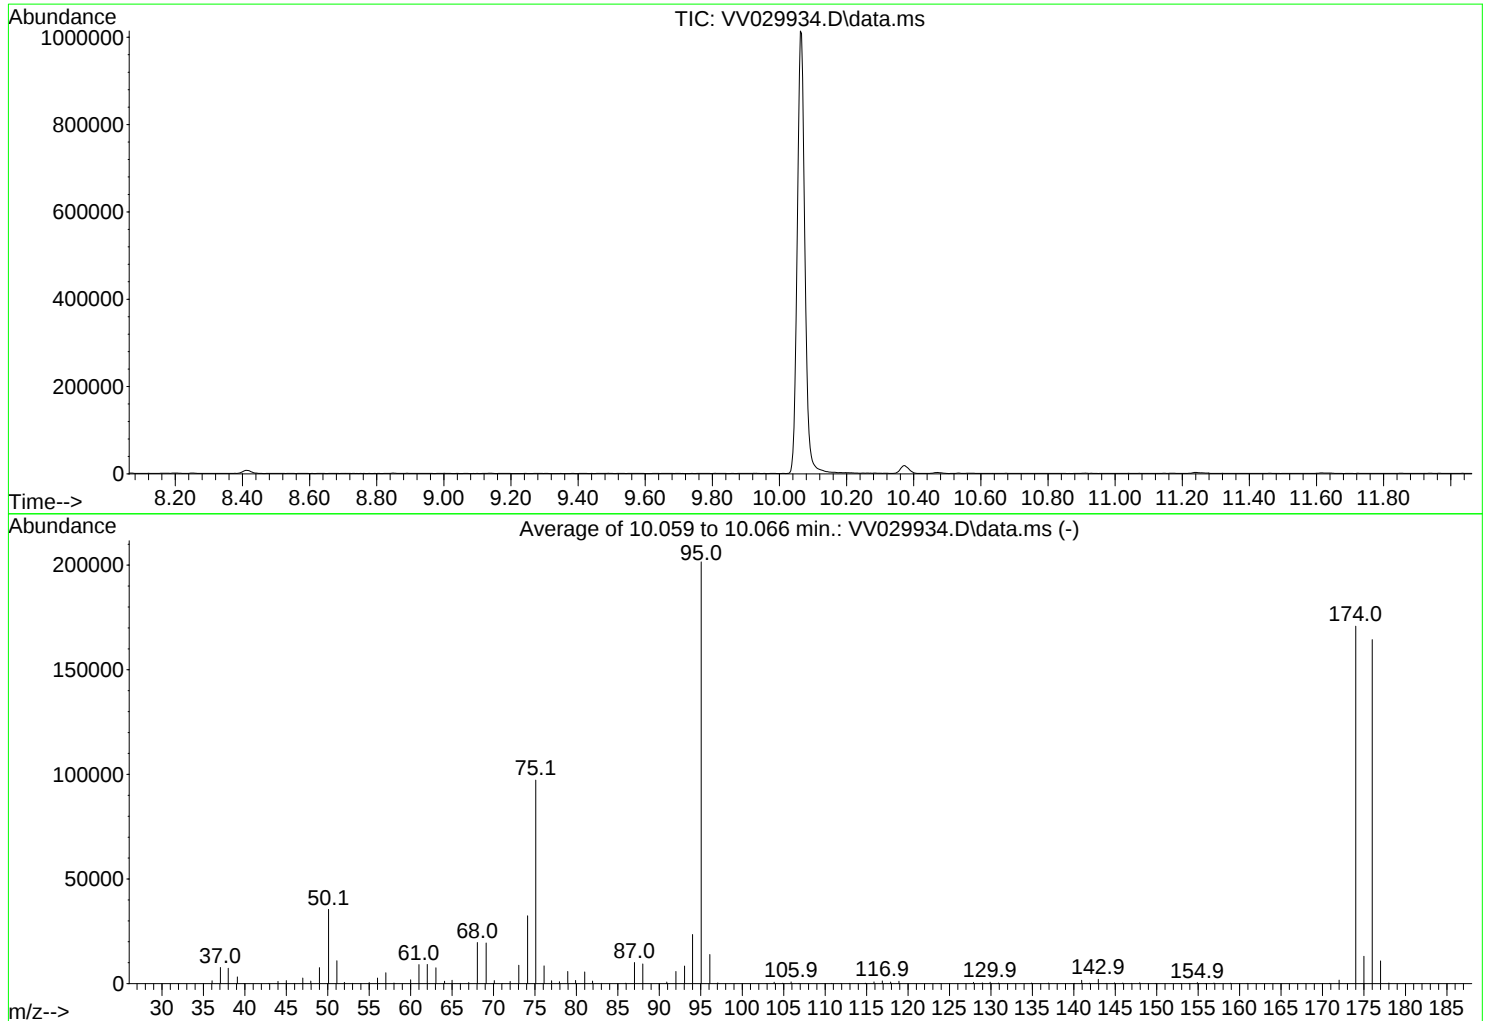

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	35477	PASS
75	95	30	80	48.2	97245	PASS
95	95	100	100	100.0	201579	PASS
96	95	5	9	6.9	13938	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.8	170859	PASS
175	174	5	9	7.7	13105	PASS
176	174	95	105	96.2	164395	PASS
177	176	5	10	6.6	10858	PASS

m/z	Abundance
39.90	396.0
44.00	476.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
36.10	1371.0
37.00	7348.0
38.00	7100.0
39.10	3222.0
40.00	462.0
42.90	159.0
44.00	1415.0
45.00	1308.0
45.90	160.0
47.00	2518.0
48.00	1224.0
49.00	7472.0
50.10	33416.0
51.10	10505.0
52.00	616.0
53.00	168.0
55.00	469.0
56.00	2598.0
57.00	4873.0
58.00	264.0
60.00	1702.0
61.00	8770.0
62.00	8626.0
63.00	7207.0
64.10	1145.0
65.00	1530.0
66.00	155.0
67.00	596.0
68.10	18568.0
69.10	18488.0
70.10	1422.0
71.10	111.0
72.00	1017.0
73.00	8347.0
74.10	31144.0
75.10	91288.0
76.10	8093.0
77.00	1192.0
77.90	821.0
79.00	5407.0
79.90	1479.0
81.00	5329.0
82.00	1144.0
83.10	114.0
85.90	222.0
87.00	9463.0
88.00	8690.0
90.90	804.0
92.00	5528.0
93.00	7876.0
94.00	21944.0
95.10	189184.0
96.10	13404.0
97.10	416.0
102.90	121.0
103.90	607.0
104.90	285.0
105.90	734.0
106.90	164.0
110.80	162.0
111.90	157.0
112.90	129.0
114.90	248.0
115.90	753.0
116.90	1138.0
117.90	667.0
118.90	1094.0
123.90	108.0
127.90	576.0
129.00	323.0
129.90	697.0
130.90	268.0
134.90	309.0
137.00	253.0
140.10	158.0
141.00	1483.0
141.90	223.0
142.90	1929.0
143.90	153.0
144.90	375.0
145.90	268.0
146.90	147.0
147.90	370.0
149.00	116.0
149.80	154.0
152.90	154.0
153.90	109.0
154.90	518.0
155.90	100.0
156.90	294.0
158.90	207.0
160.90	159.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

170.90	195.0
172.00	1495.0
174.00	157056.0
175.00	12354.0
176.00	151744.0
177.00	10197.0
178.10	309.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
36.10	1473.0
37.00	7995.0
38.00	7568.0
39.10	3254.0
39.90	453.0
42.90	180.0
44.00	1568.0
45.00	1505.0
46.00	195.0
47.00	2800.0
47.90	1293.0
49.00	7939.0
50.10	36768.0
51.10	11322.0
52.00	648.0
53.00	162.0
54.00	108.0
55.00	547.0
56.00	2809.0
57.00	5483.0
58.00	282.0
60.00	1922.0
61.00	9461.0
62.00	9501.0
63.10	7890.0
64.10	1216.0
65.00	1715.0
66.00	152.0
67.00	536.0
68.10	20520.0
69.10	20040.0
70.10	1482.0
71.10	107.0
72.00	1087.0
73.10	9070.0
74.10	33592.0
75.10	100704.0
76.10	8769.0
77.00	1461.0
77.90	926.0
78.90	6063.0
79.90	1554.0
81.00	5777.0
81.90	1239.0
83.10	120.0
85.90	249.0
87.00	10489.0
88.00	9780.0
90.90	786.0
92.00	6043.0
93.00	8627.0
94.00	24248.0
95.00	208512.0
96.10	14485.0
97.10	417.0
102.90	109.0
103.80	702.0
104.90	276.0
105.90	829.0
106.80	181.0
110.80	182.0
111.90	165.0
112.90	126.0
114.90	269.0
115.90	900.0
116.90	1348.0
117.90	790.0
118.90	1172.0
123.80	103.0
127.90	613.0
129.00	406.0
129.90	746.0
130.90	295.0
134.90	343.0
136.90	288.0
140.10	187.0
140.90	1680.0
141.90	233.0
142.90	2131.0
143.90	186.0
144.90	394.0
145.90	296.0
147.00	151.0
148.00	451.0
149.00	112.0
149.90	178.0
152.90	145.0
153.90	129.0
154.90	577.0
156.90	349.0
158.90	256.0
160.90	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

170.80	196.0
172.00	1693.0
174.00	176576.0
175.00	13605.0
176.00	170304.0
177.00	11235.0
178.00	341.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
36.00	1378.0
37.10	7792.0
38.00	7358.0
39.10	3065.0
39.90	477.0
42.90	173.0
44.00	1632.0
45.00	1538.0
46.00	217.0
47.00	2774.0
47.90	1250.0
49.00	7649.0
50.10	36248.0
51.10	11078.0
52.00	581.0
53.00	130.0
54.00	101.0
55.00	585.0
56.00	2687.0
57.00	5331.0
58.00	275.0
60.00	1958.0
61.00	9013.0
62.00	9355.0
63.10	7723.0
64.10	1109.0
65.00	1647.0
66.00	139.0
67.00	456.0
68.00	19984.0
69.10	19736.0
70.10	1453.0
72.00	1066.0
73.10	8871.0
74.10	32600.0
75.10	99744.0
76.10	8636.0
77.00	1547.0
78.00	974.0
79.00	6068.0
79.90	1527.0
81.00	5741.0
81.90	1194.0
83.00	133.0
86.00	265.0
87.00	10442.0
88.00	9837.0
90.90	735.0
92.00	5891.0
93.10	8684.0
94.00	24200.0
95.00	207040.0
96.10	13926.0
97.00	400.0
103.80	750.0
104.90	234.0
105.90	861.0
106.90	210.0
110.80	157.0
111.90	151.0
112.90	109.0
114.80	268.0
115.90	855.0
116.90	1427.0
117.90	826.0
118.90	1135.0
123.80	122.0
127.90	624.0
128.90	409.0
129.90	686.0
130.90	301.0
134.90	336.0
136.90	320.0
140.00	207.0
140.90	1724.0
141.90	192.0
143.00	2216.0
143.90	164.0
144.90	411.0
145.90	301.0
147.00	138.0
148.00	473.0
150.00	191.0
152.90	109.0
153.90	135.0
154.90	527.0
156.90	370.0
158.90	266.0
160.90	171.0
170.80	186.0
172.00	1792.0
174.00	178944.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

175.00	13357.0
176.00	171136.0
177.00	11143.0
177.90	343.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216