
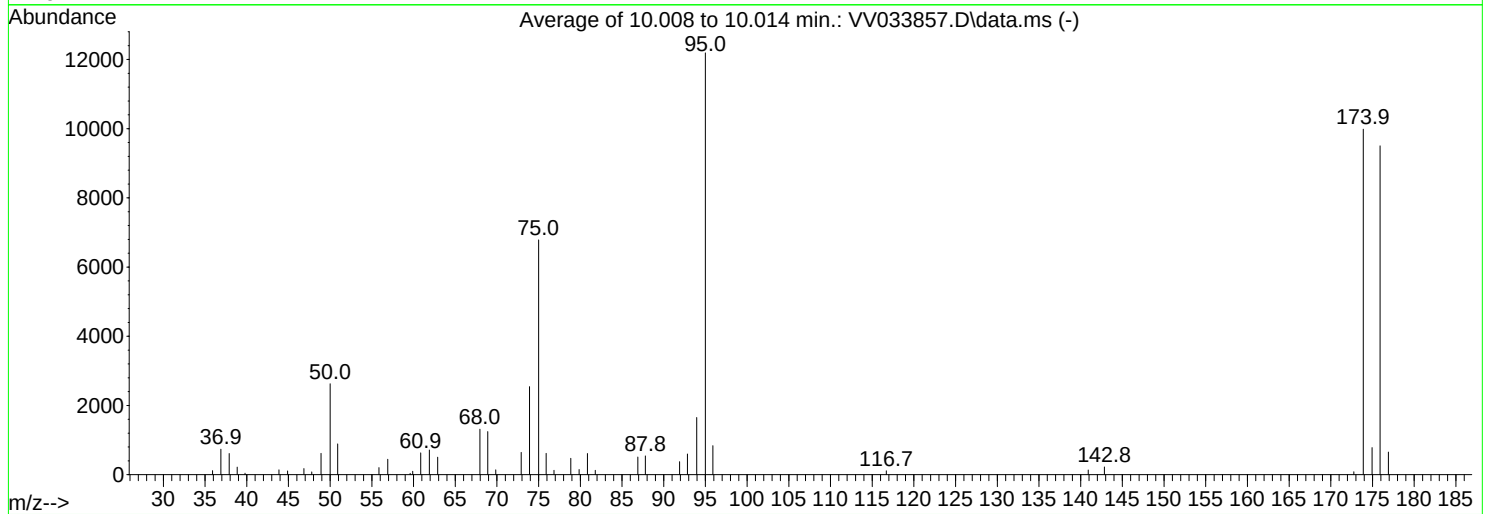


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012524\
Data File : VV033857.D
Acq On : 25 Jan 2024 08:32
Operator : SY/MD
Sample : BFB242
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB242

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 25 21:12:54 2024

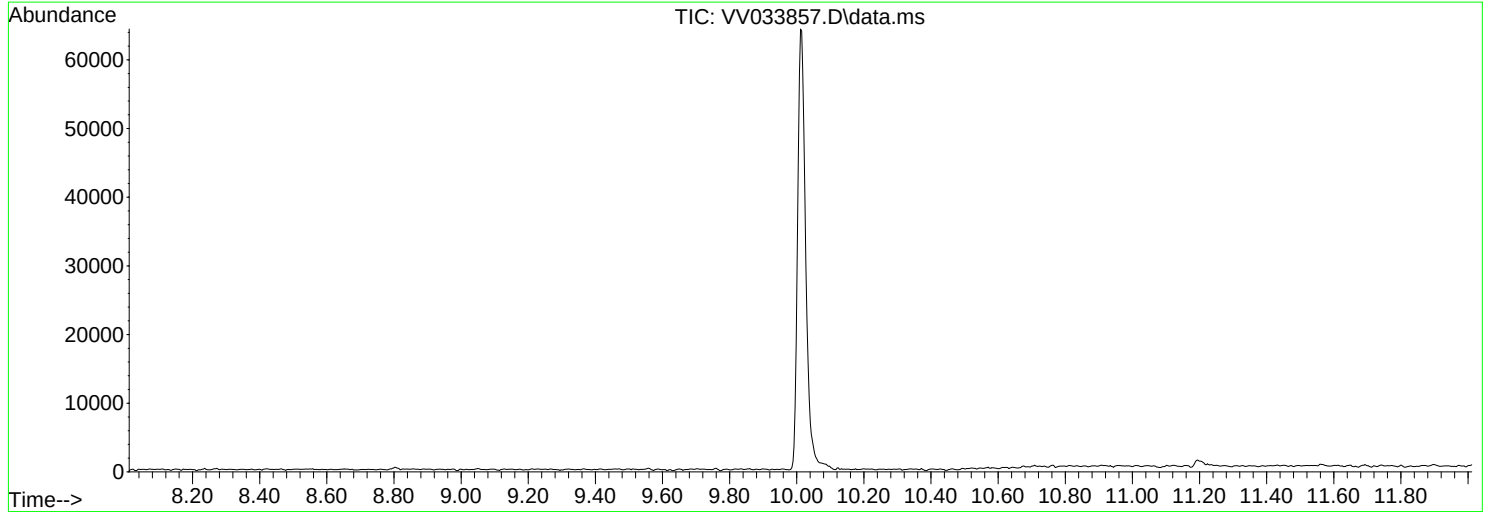

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	2627	PASS
75	95	30	80	55.7	6786	PASS
95	95	100	100	100.0	12191	PASS
96	95	5	9	6.9	839	PASS
173	174	0.00	2	0.8	84	PASS
174	95	50	120	81.9	9985	PASS
175	174	5	9	7.9	784	PASS
176	174	95	105	95.2	9504	PASS
177	176	5	10	6.9	653	PASS

m/z	Abundance
39.90	181.0
43.80	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
36.00	125.0
36.90	678.0
37.90	585.0
38.80	213.0
39.80	226.0
43.90	258.0
44.80	105.0
46.80	137.0
47.80	118.0
48.90	607.0
50.00	2627.0
50.90	914.0
55.90	186.0
56.90	430.0
59.60	116.0
60.80	609.0
61.90	693.0
62.90	467.0
67.90	1210.0
68.90	1076.0
69.80	133.0
72.90	591.0
73.90	2446.0
75.00	6475.0
75.90	527.0
76.90	120.0
78.80	479.0
80.00	133.0
80.90	618.0
81.80	125.0
86.90	556.0
87.80	557.0
91.90	335.0
92.80	557.0
94.00	1542.0
95.00	11286.0
95.90	866.0
116.70	122.0
140.80	128.0
142.90	202.0
172.70	114.0
173.90	8875.0
175.00	677.0
175.90	8511.0
176.90	581.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
35.90	111.0
36.90	782.0
37.90	635.0
38.90	228.0
39.80	215.0
43.90	252.0
44.90	104.0
46.80	181.0
47.80	119.0
48.90	654.0
50.00	2733.0
50.90	928.0
55.80	206.0
56.90	456.0
59.90	132.0
60.90	625.0
61.90	730.0
62.90	519.0
68.00	1352.0
68.90	1262.0
69.80	143.0
72.90	667.0
73.90	2641.0
75.00	7005.0
75.90	630.0
76.90	119.0
78.80	494.0
79.80	145.0
80.80	631.0
81.80	126.0
86.90	532.0
87.80	565.0
91.90	384.0
92.90	620.0
93.90	1717.0
95.00	12666.0
95.90	880.0
116.70	117.0
140.90	128.0
142.90	237.0
172.80	137.0
173.90	10345.0
175.00	802.0
175.90	9858.0
176.90	683.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
35.90	110.0
36.90	751.0
37.90	610.0
38.90	208.0
39.90	221.0
43.90	240.0
45.00	109.0
46.90	203.0
48.90	583.0
50.00	2522.0
50.90	824.0
55.90	216.0
56.90	452.0
59.90	161.0
60.90	655.0
61.90	714.0
62.90	522.0
67.90	1379.0
68.90	1388.0
69.90	139.0
72.90	665.0
73.90	2546.0
75.00	6879.0
75.90	691.0
76.80	131.0
78.90	440.0
79.80	170.0
80.80	583.0
81.80	123.0
86.90	446.0
87.80	503.0
91.90	405.0
92.90	615.0
93.90	1698.0
95.00	12620.0
95.90	772.0
116.70	100.0
141.00	140.0
142.80	223.0
173.90	10736.0
174.90	873.0
175.90	10144.0
176.90	694.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242