
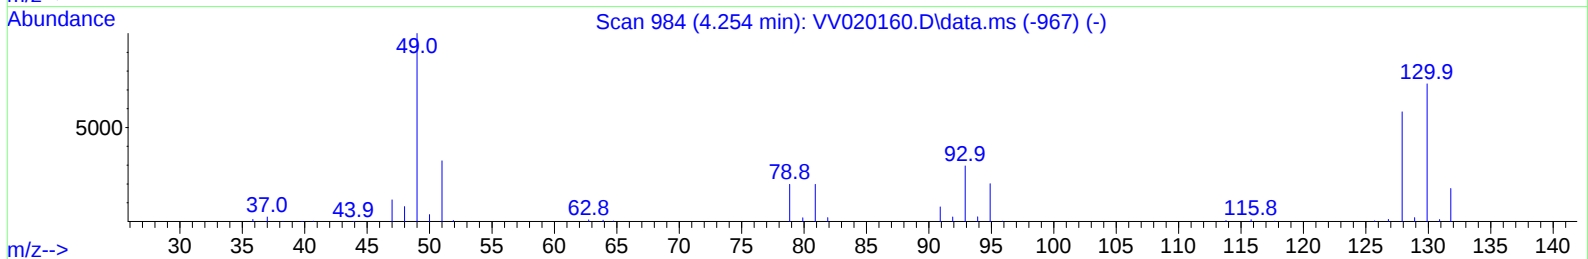
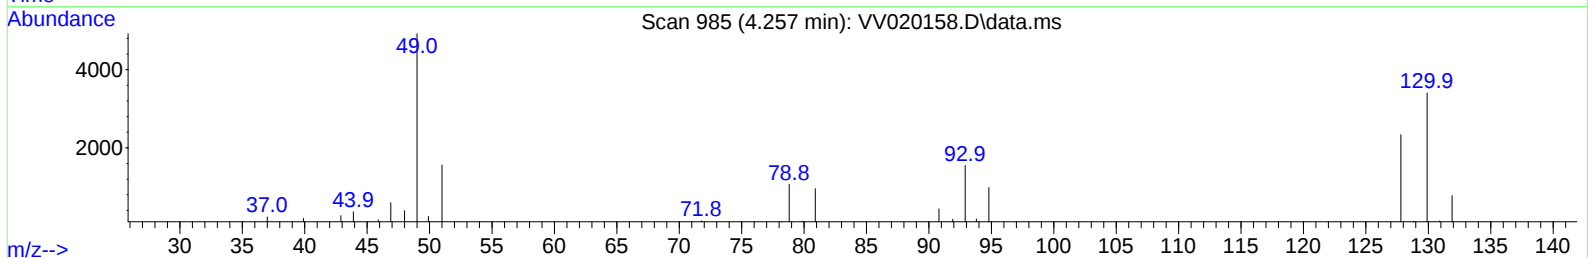


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
Data File : VV020158.D
Acq On : 25 Jan 2021 16:19
Operator : SY/MD
Sample : VSTD00561
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 17:45:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 25 17:43:44 2021
Response via : Initial Calibration

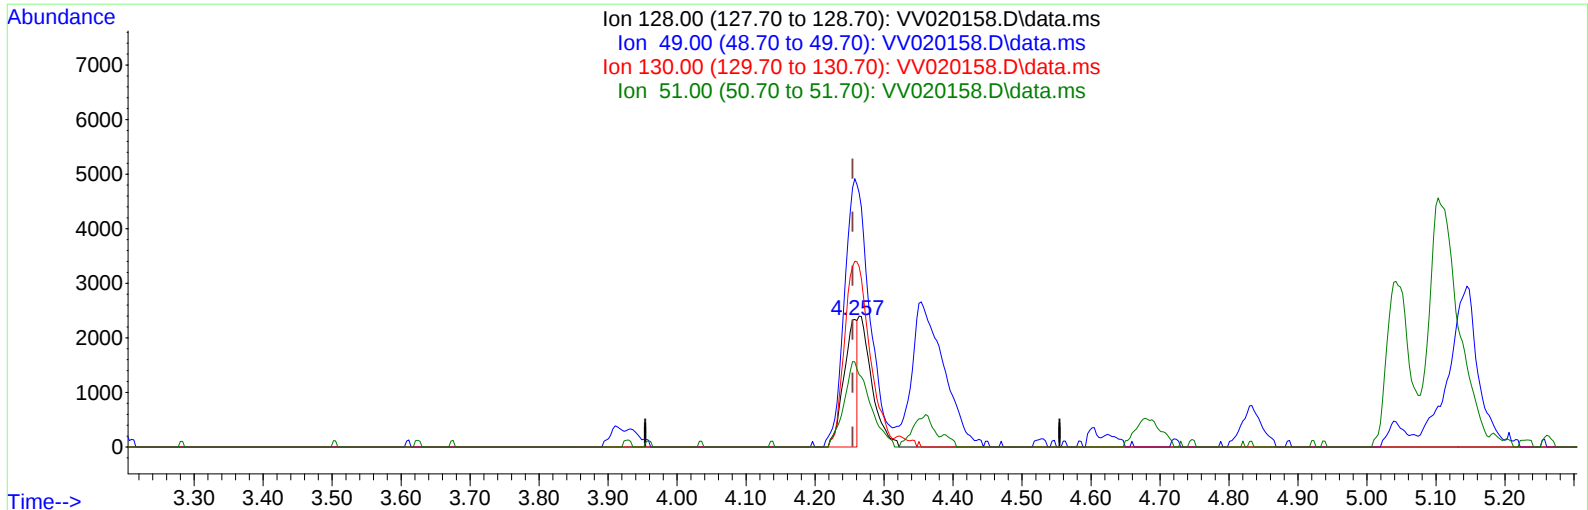

TIC: VV020158.D\data.ms

(23) Bromochloromethane (T)

4.257min (+ 0.003) 1.83 ug/L

response 3169

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	155.50	210.44#
130.00	126.40	145.61
51.00	47.20	66.80#