
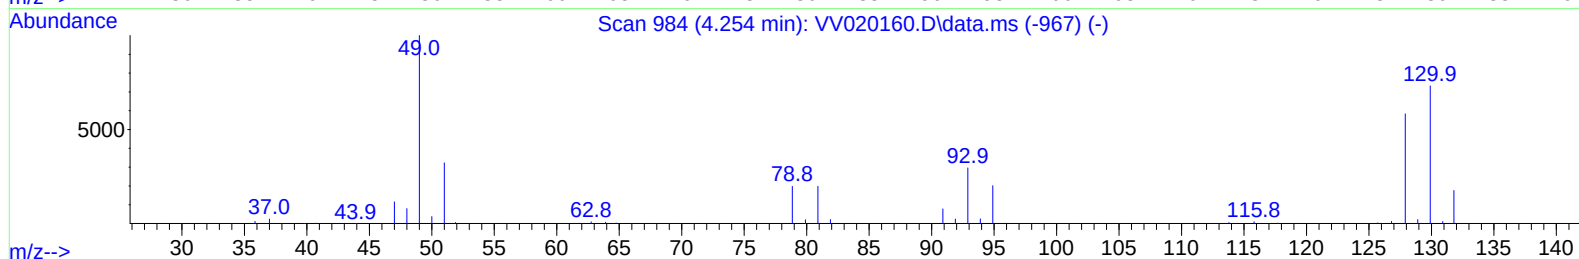
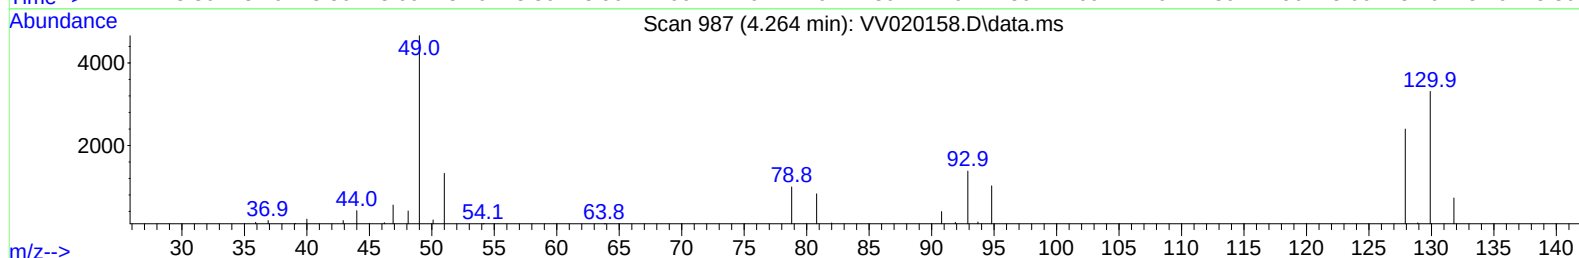


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
 Data File : VV020158.D
 Acq On : 25 Jan 2021 16:19
 Operator : SY/MD
 Sample : VSTD00561
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 17:45:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 25 17:43:44 2021
 Response via : Initial Calibration

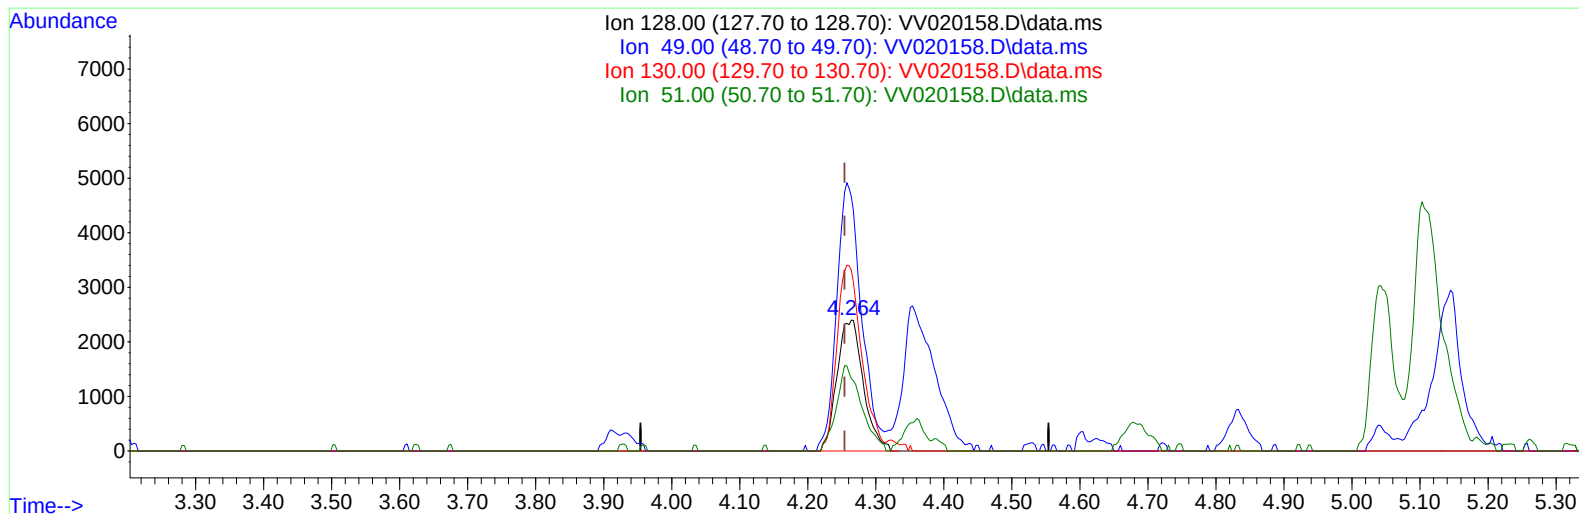

TIC: VV020158.D\data.ms

(23) Bromochloromethane (T)

4.264min (+ 0.010) 3.72 ug/L m

response 6444

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	155.50	194.13
130.00	126.40	137.88
51.00	47.20	55.25