




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
Data File : VV020166.D
Acq On : 25 Jan 2021 22:18
Operator : SY/MD
Sample : L5214-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT1-2021-01

Manual Integrations
APPROVED

MMDadoda
1/29/2021 11:56:56 AM

Quant Time: Jan 26 06:23:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 25 18:17:01 2021
Response via : Initial Calibration

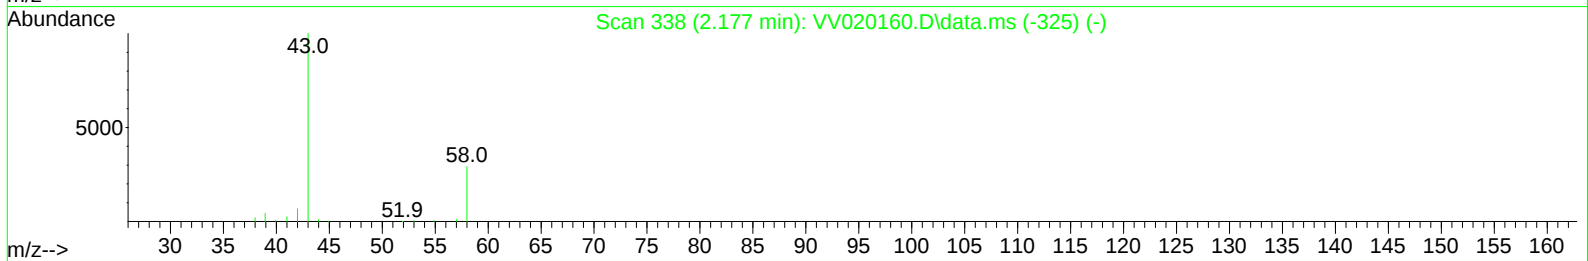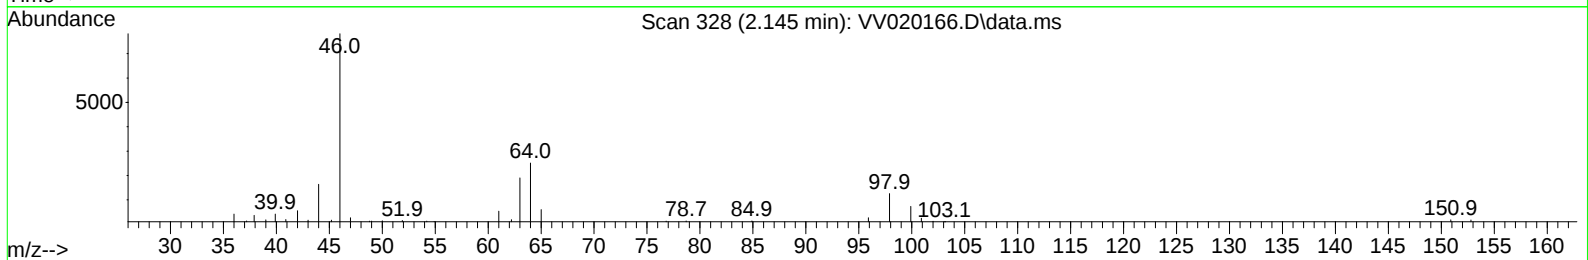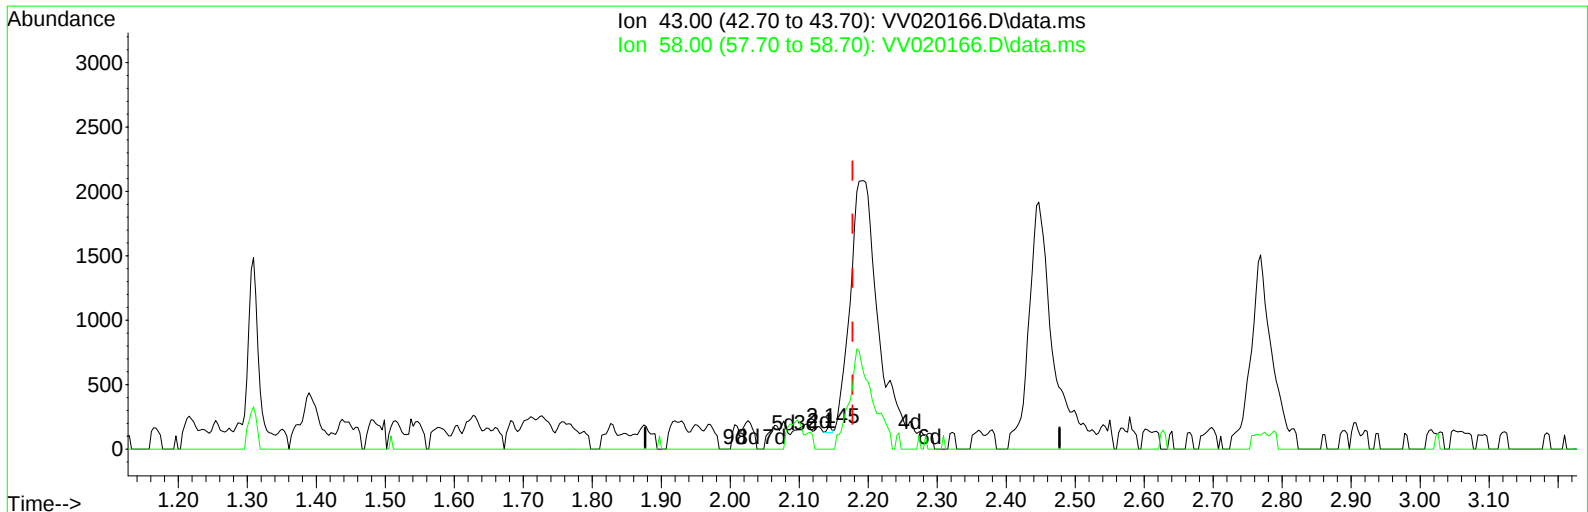

TIC: VV020166.D\data.ms

(13) Acetone (T)

2.145min (-0.032) 0.01 ug/L

response	19	
Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.90	8173.68#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
Data File : VV020166.D
Acq On : 25 Jan 2021 22:18
Operator : SY/MD
Sample : L5214-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT1-2021-01

Manual Integrations
APPROVED

MMDadoda
1/29/2021 11:56:56 AM

Quant Time: Jan 26 06:23:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 25 18:17:01 2021
Response via : Initial Calibration

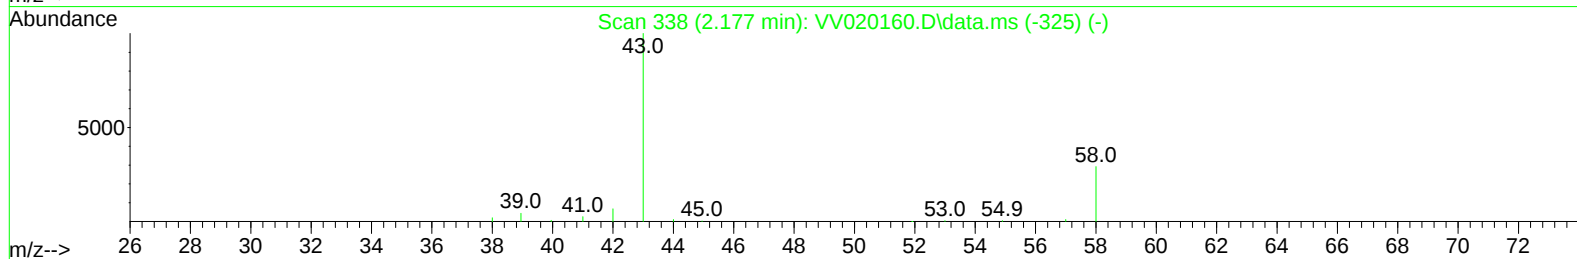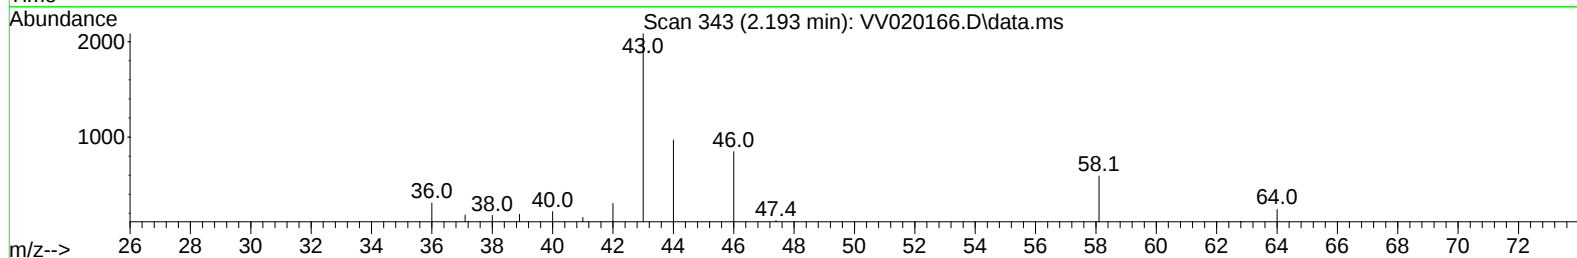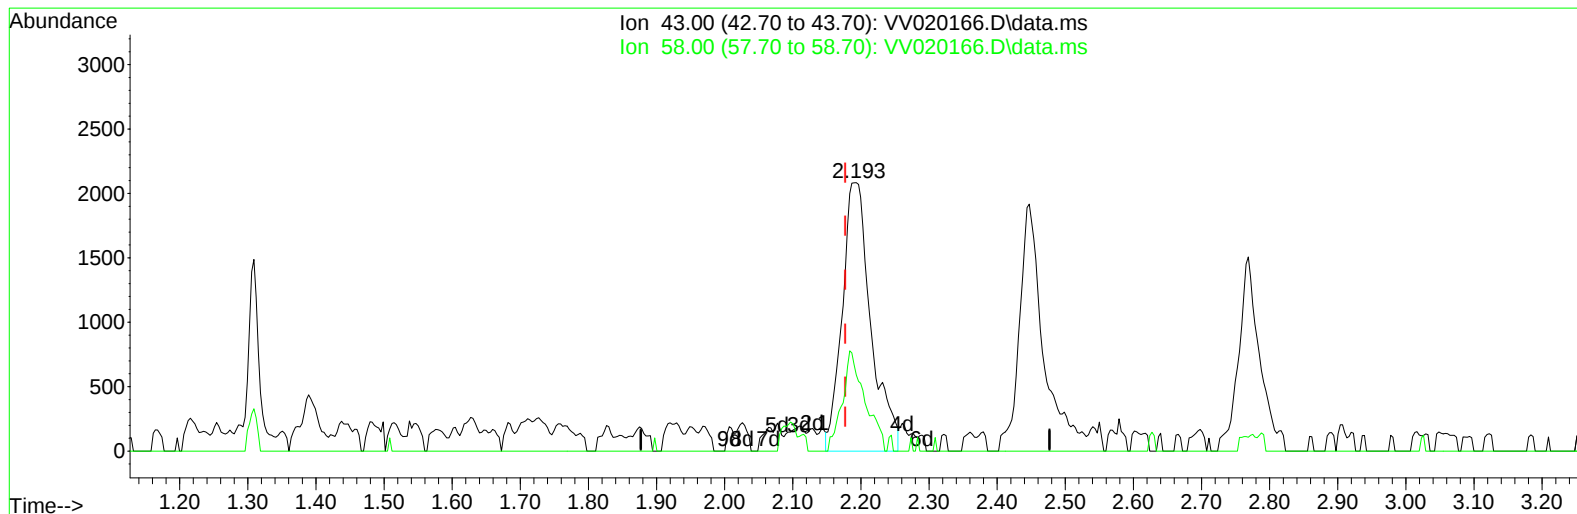

TIC: VV020166.D\data.ms

(13) Acetone (T)

2.193min (+ 0.016) 4.04 ug/L m

response 6095

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.90	25.48
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
 Data File : VV020166.D
 Acq On : 25 Jan 2021 22:18
 Operator : SY/MD
 Sample : L5214-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-MED-SOIL-QT1-2021-01

Manual Integrations
 APPROVED

MMDadoda
 1/29/2021 11:56:56 AM

Quant Time: Jan 26 06:23:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 25 18:17:01 2021
 Response via : Initial Calibration

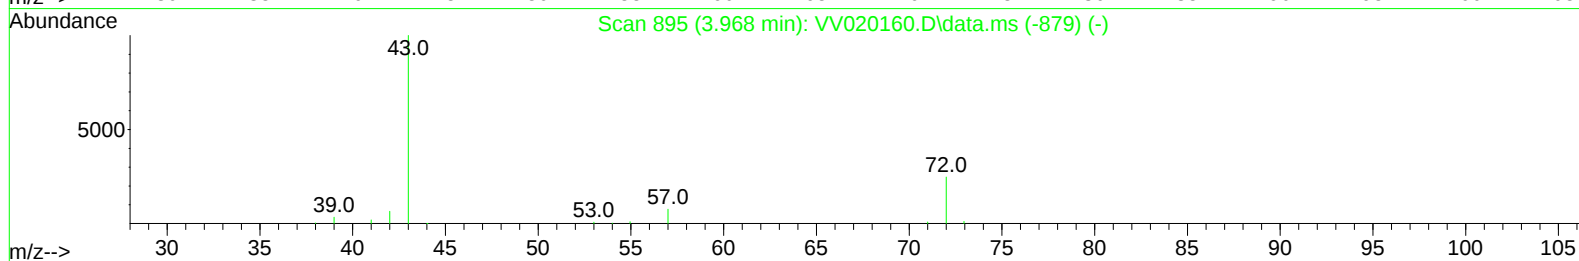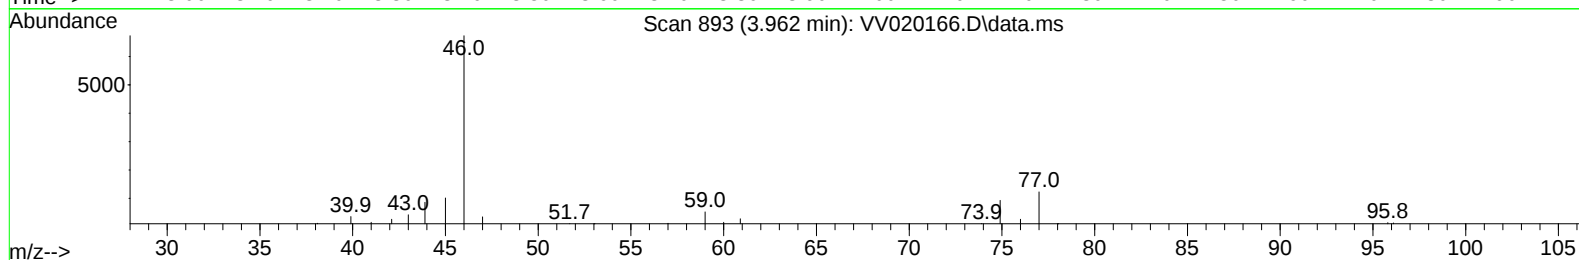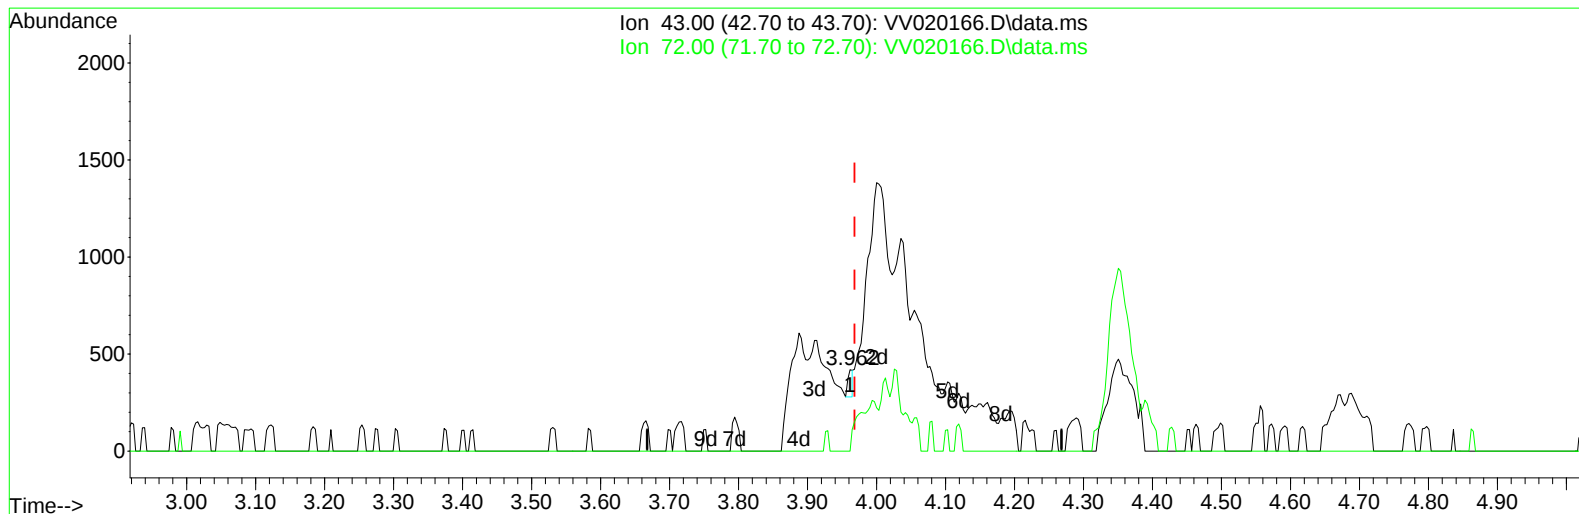

TIC: VV020166.D\data.ms

(22) 2-Butanone (T)

3.962min (-0.006) 0.04 ug/L

response

71

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.30	330.99#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
Data File : VV020166.D
Acq On : 25 Jan 2021 22:18
Operator : SY/MD
Sample : L5214-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT1-2021-01

Manual Integrations
APPROVED

MMDadoda
1/29/2021 11:56:56 AM

Quant Time: Jan 26 06:23:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 25 18:17:01 2021
Response via : Initial Calibration

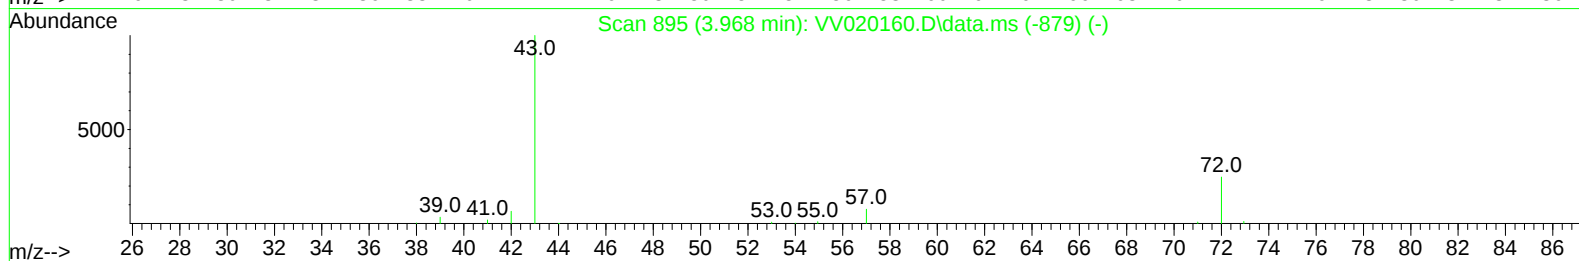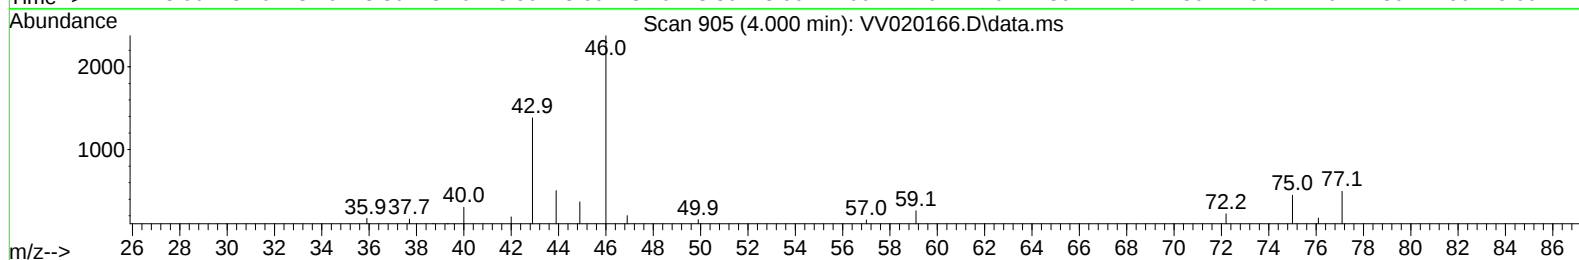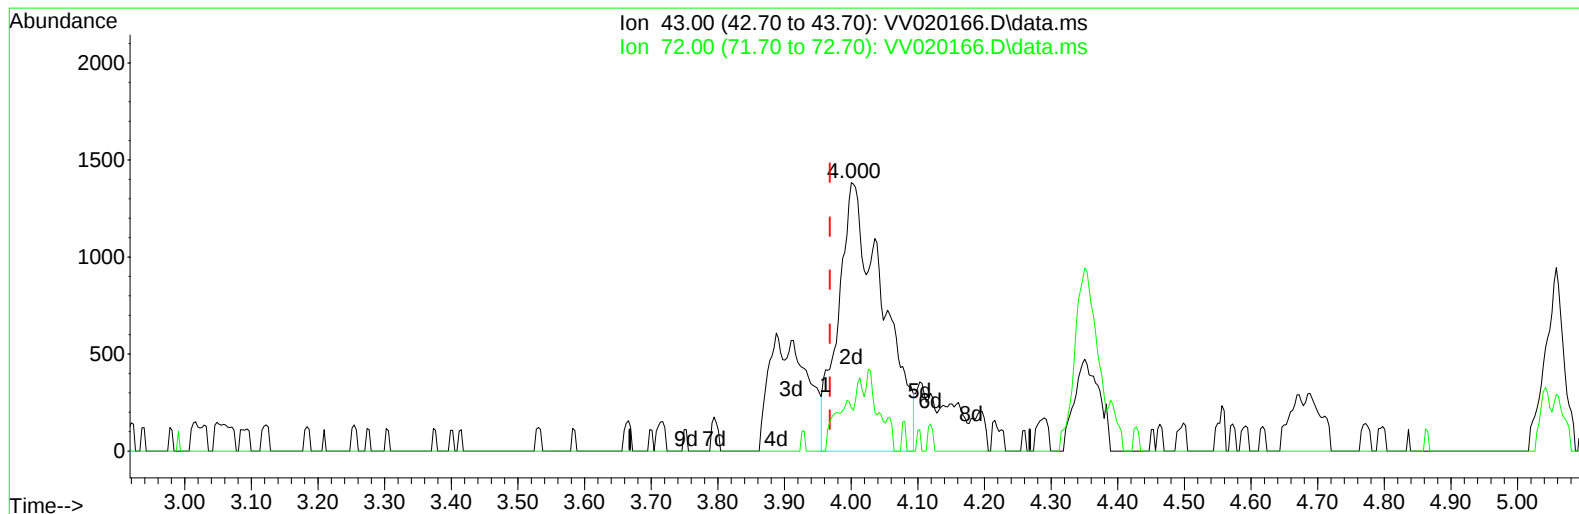

TIC: VV020166.D\data.ms

(22) 2-Butanone (T)

4.000min (+ 0.032) 3.15 ug/L m

response 6383

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.30	3.68#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
Data File : VV020166.D
Acq On : 25 Jan 2021 22:18
Operator : SY/MD
Sample : L5214-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT1-2021-01

Manual Integrations
APPROVED

MMDadoda
1/29/2021 11:56:56 AM

Quant Time: Jan 26 06:23:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 25 18:17:01 2021
Response via : Initial Calibration

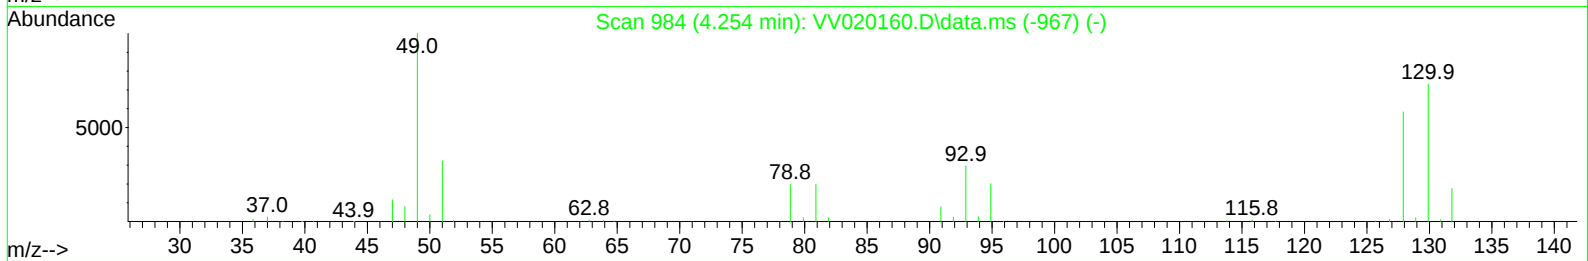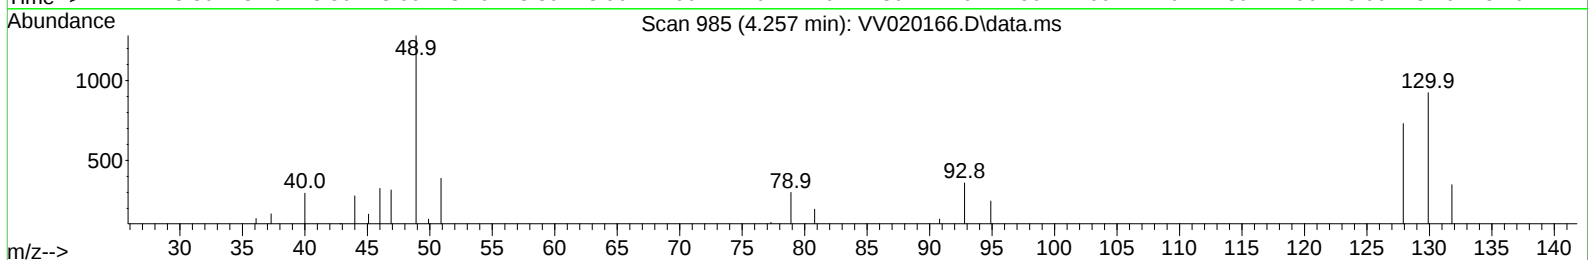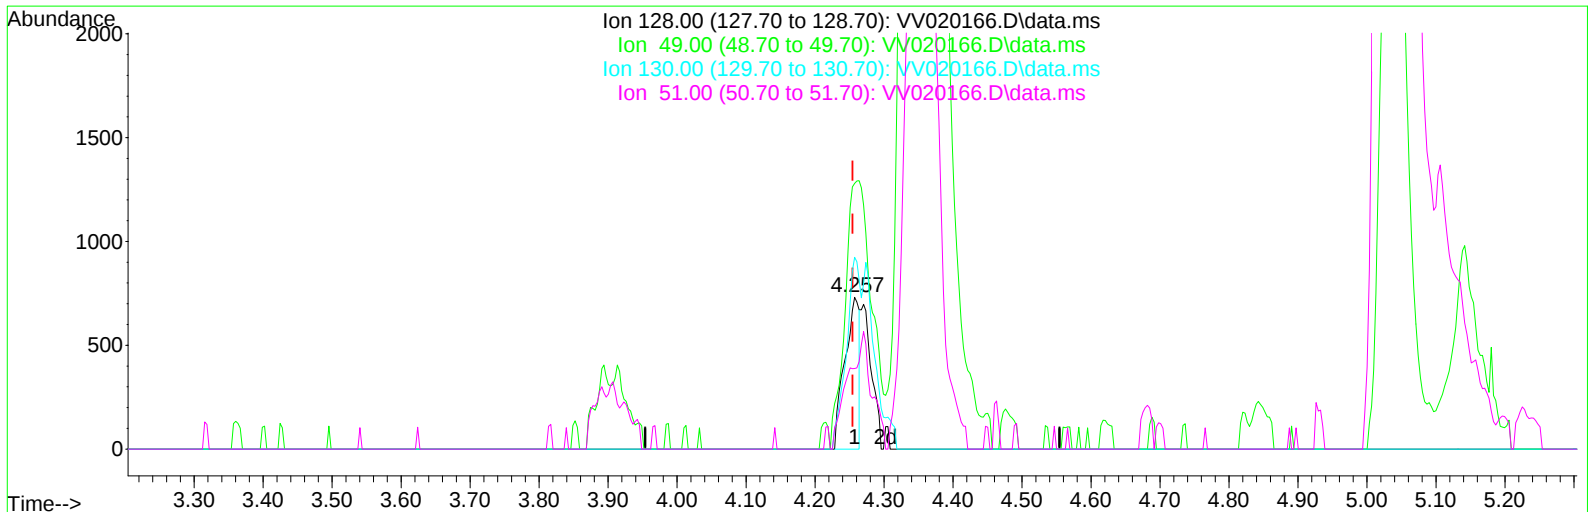

TIC: VV020166.D\data.ms

(23) Bromochloromethane (T)

4.257min (+ 0.003) 0.77 ug/L

response 1058

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	155.50	175.10
130.00	126.40	126.40
51.00	47.20	53.08




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
Data File : VV020166.D
Acq On : 25 Jan 2021 22:18
Operator : SY/MD
Sample : L5214-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT1-2021-01

Manual Integrations
APPROVED

MMDadoda
1/29/2021 11:56:56 AM

Quant Time: Jan 26 06:23:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 25 18:17:01 2021
Response via : Initial Calibration

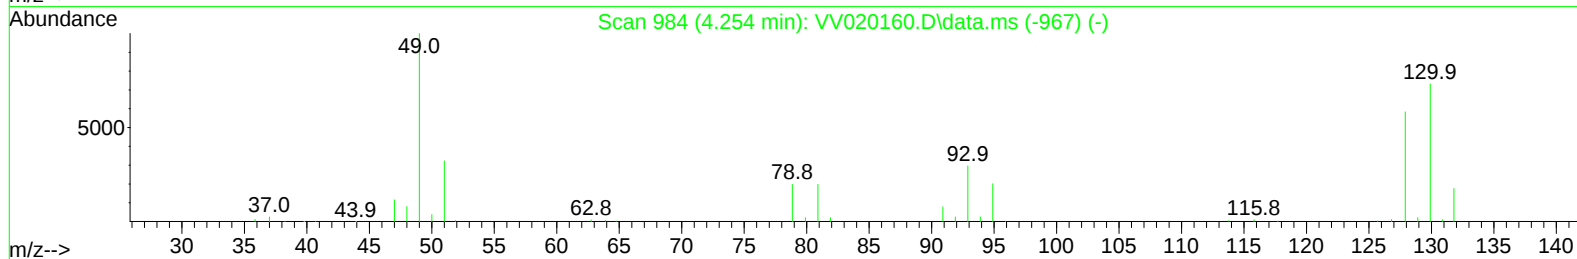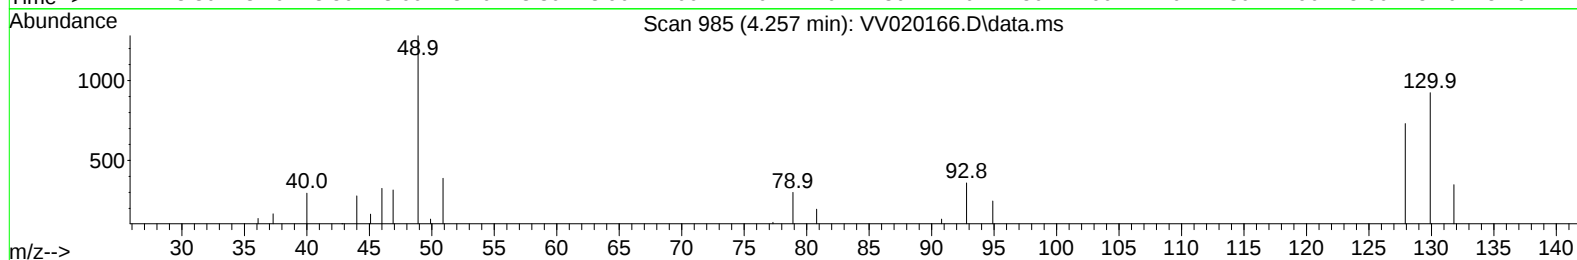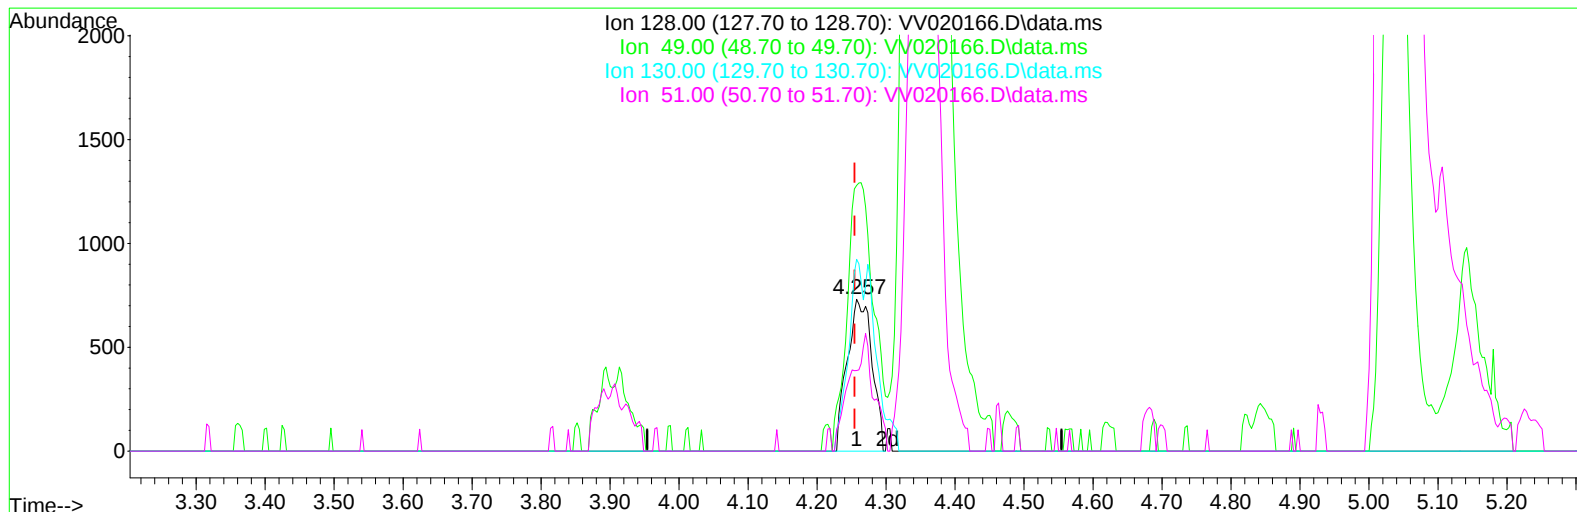

TIC: VV020166.D\data.ms

(23) Bromochloromethane (T)

4.257min (+ 0.003) 1.33 ug/L m

response 1829

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	155.50	175.10
130.00	126.40	126.40
51.00	47.20	53.08




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
Data File : VV020166.D
Acq On : 25 Jan 2021 22:18
Operator : SY/MD
Sample : L5214-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT1-2021-01

Quant Time: Jan 26 06:23:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 25 18:17:01 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
1/29/2021 11:56:56 AM

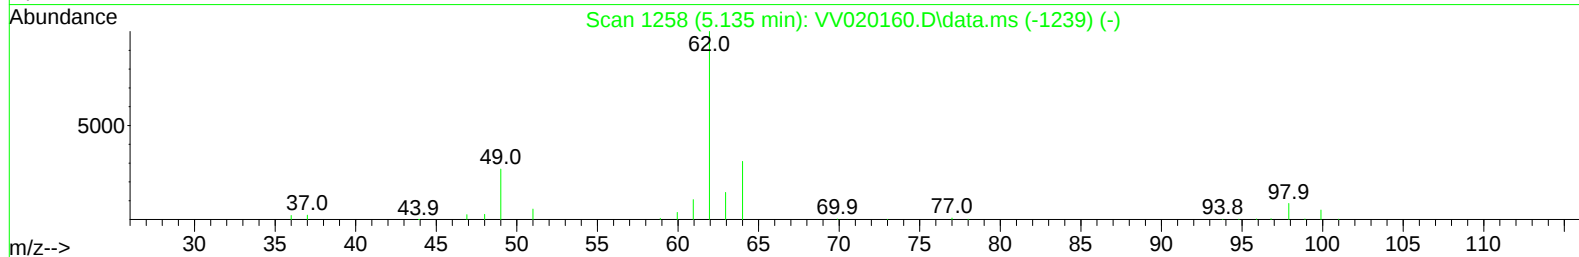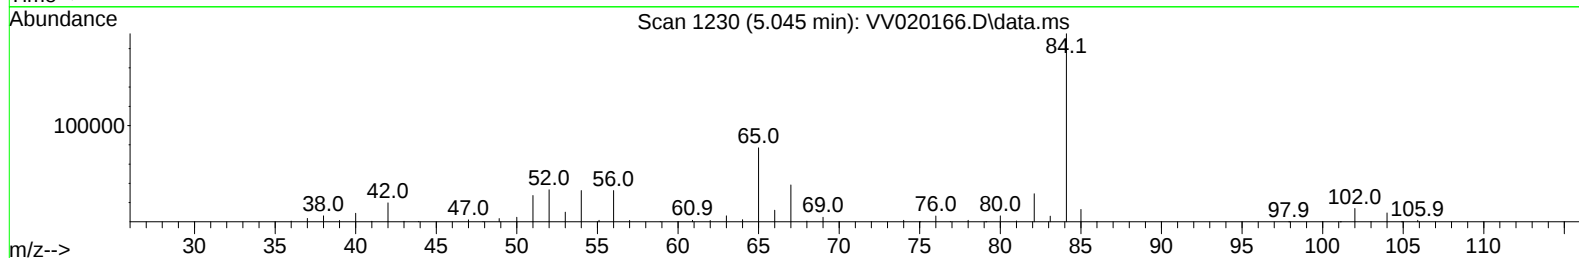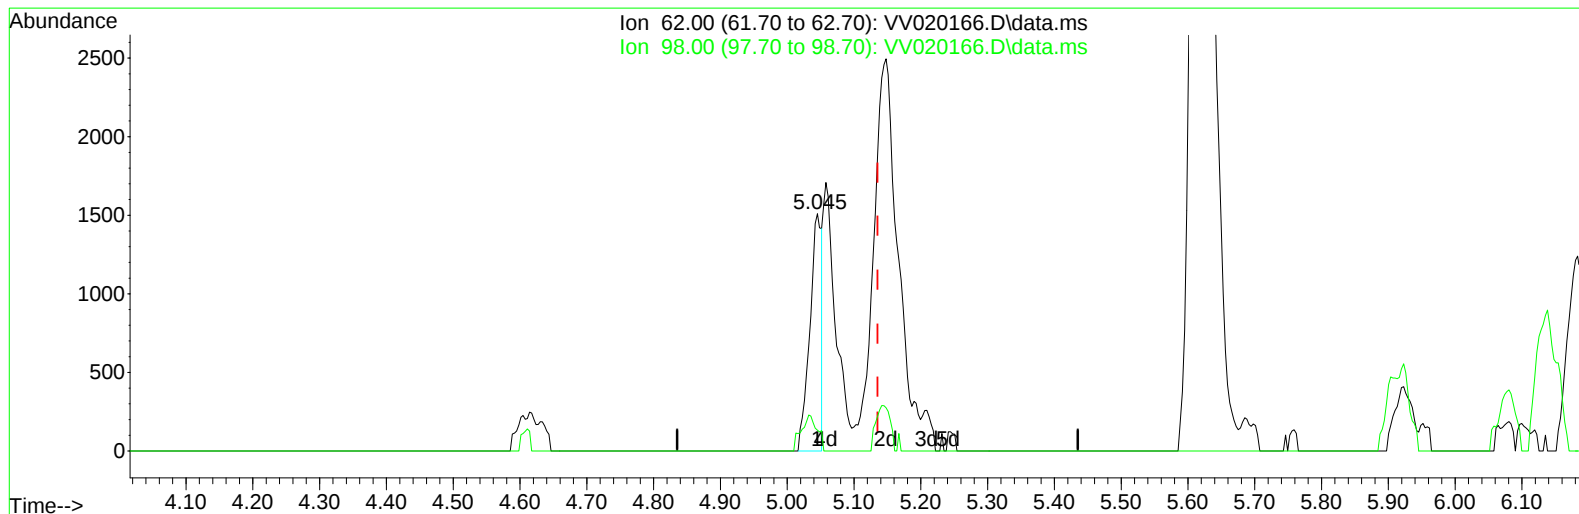

TIC: VV020166.D\data.ms

(27) 1,2-Dichloroethane (T)

5.045min (-0.090) 0.43 ug/L

response 1863

Ion	Exp%	Act%
62.00	100.00	100.00
98.00	8.50	8.74
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
 Data File : VV020166.D
 Acq On : 25 Jan 2021 22:18
 Operator : SY/MD
 Sample : L5214-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-MED-SOIL-QT1-2021-01

Manual Integrations
 APPROVED

MMDadoda
 1/29/2021 11:56:56 AM

Quant Time: Jan 26 06:23:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 25 18:17:01 2021
 Response via : Initial Calibration

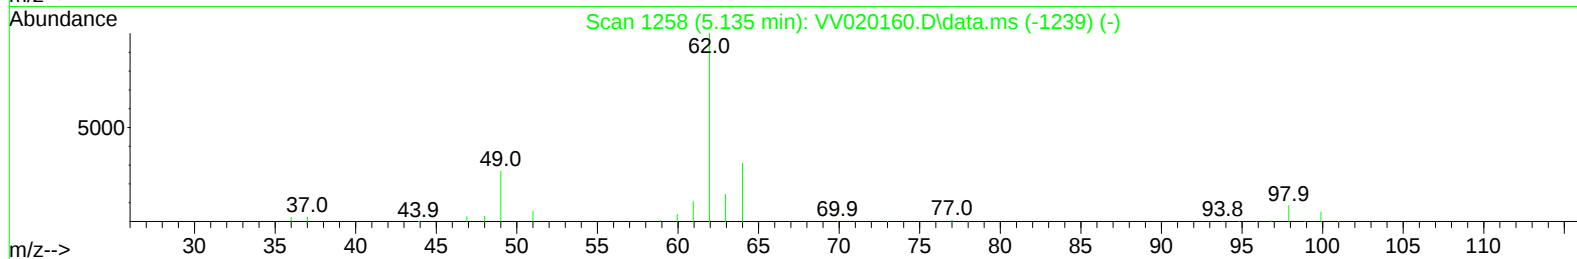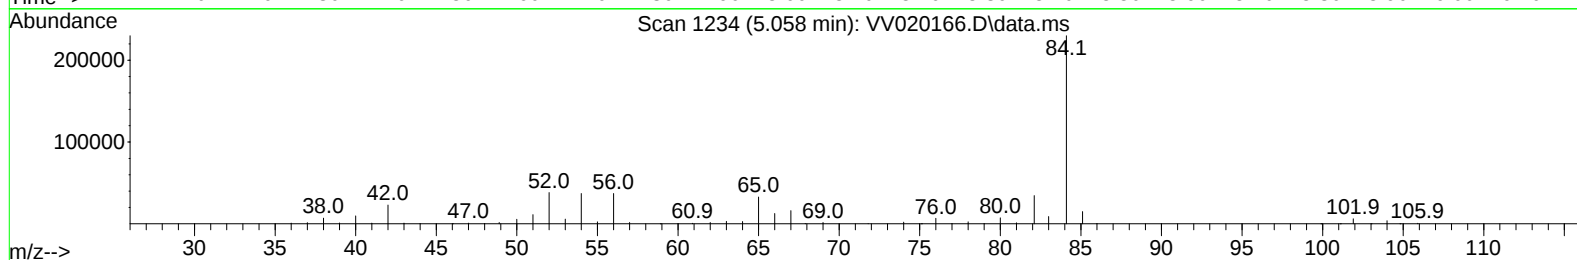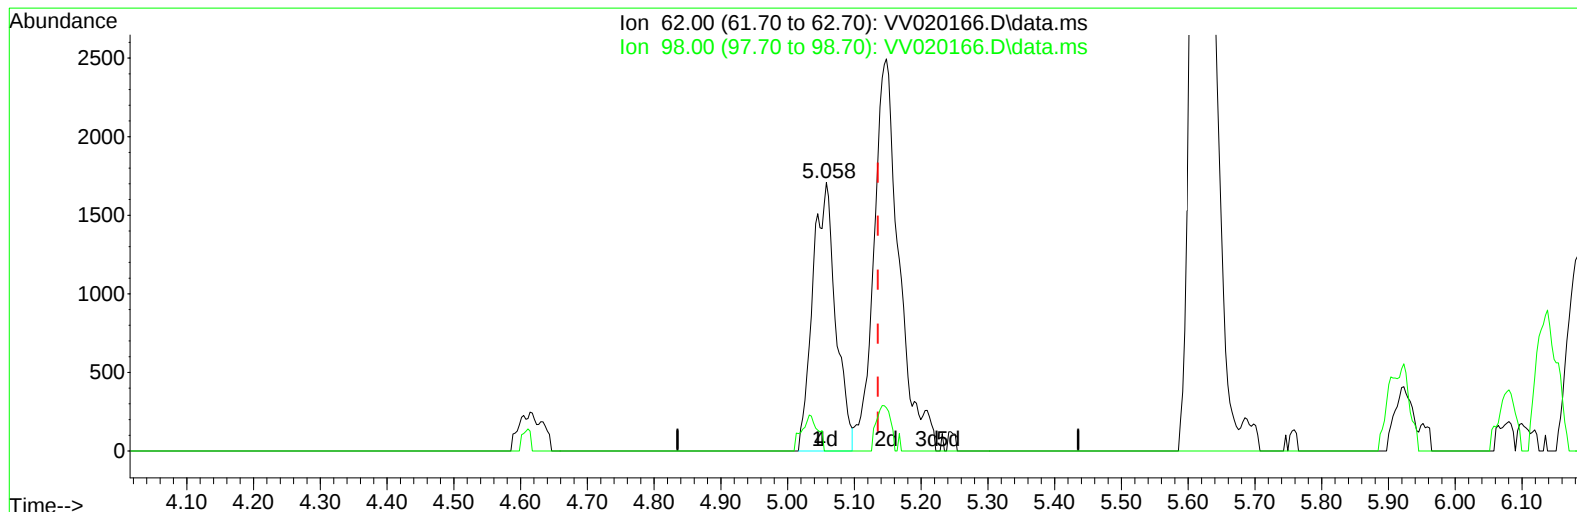

TIC: VV020166.D\data.ms

(27) 1,2-Dichloroethane (T)

5.058min (-0.077) 0.94 ug/L m

response 4078

Ion	Exp%	Act%
62.00	100.00	100.00
98.00	8.50	0.00#
0.00	0.00	0.00
0.00	0.00	0.00