




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
 Data File : VV020167.D
 Acq On : 25 Jan 2021 22:42
 Operator : SY/MD
 Sample : L5214-05
 Misc : 5.0G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-QT1-2021-01

Manual Integrations
 APPROVED

SAM
 2/1/2021 3:34:36 PM

Quant Time: Jan 26 05:50:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 25 18:17:01 2021
 Response via : Initial Calibration

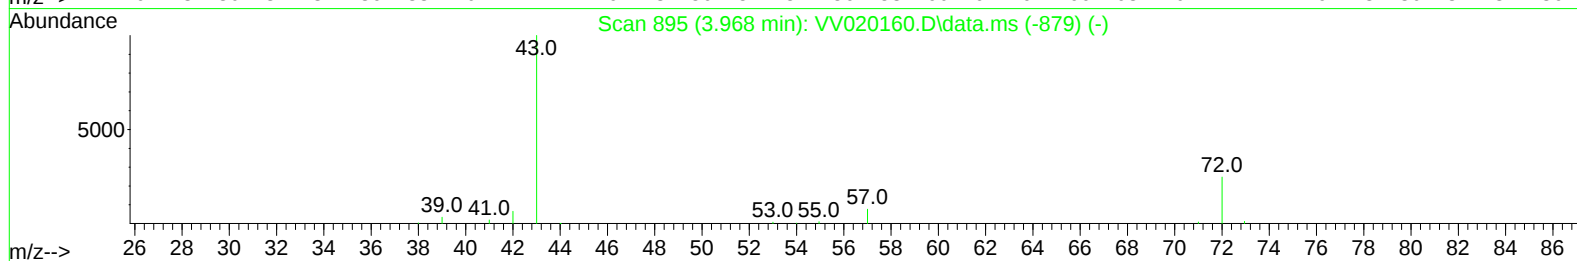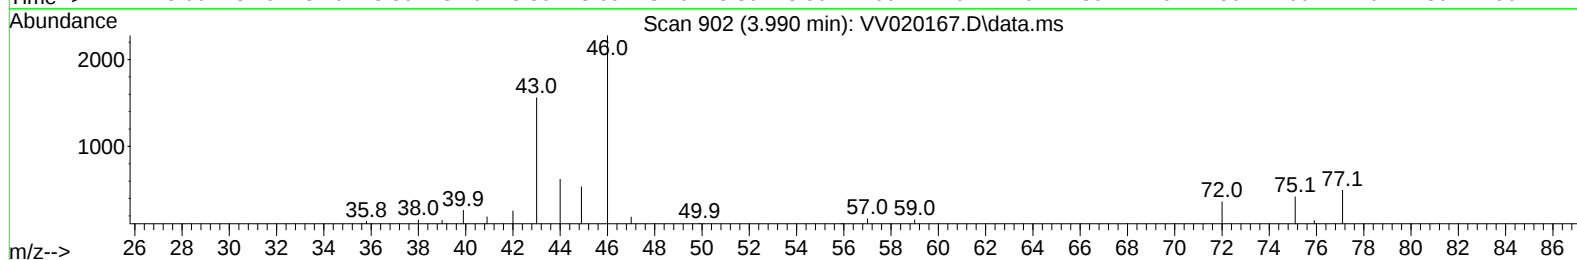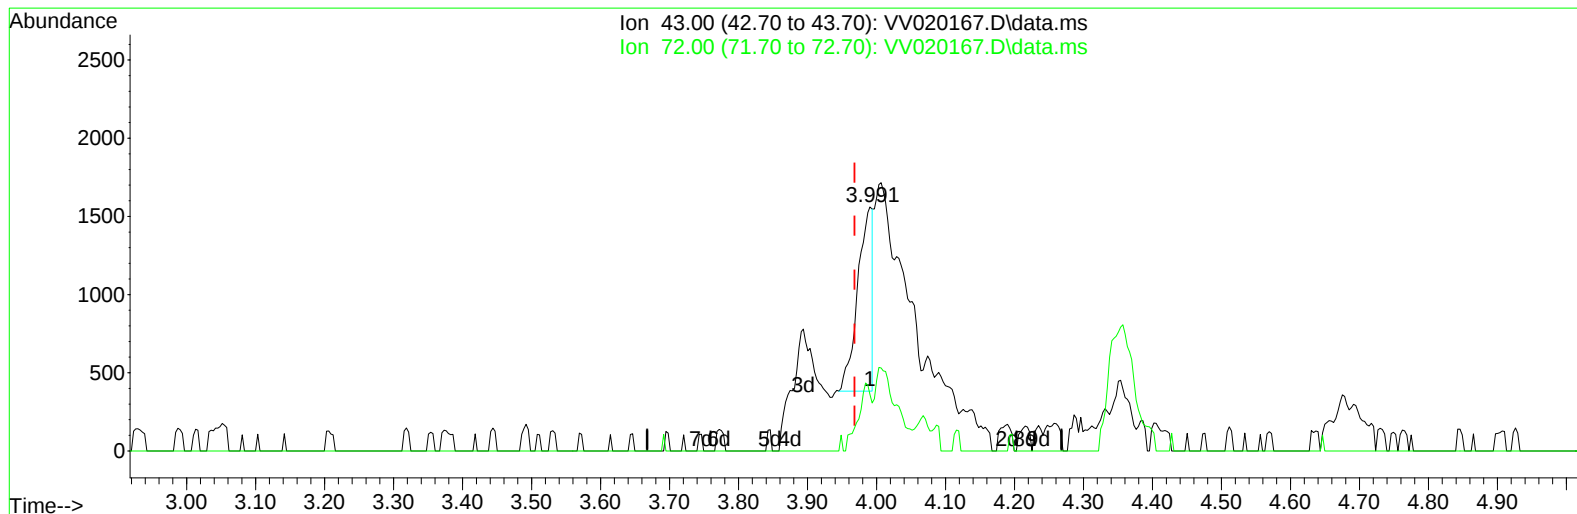

TIC: VV020167.D\data.ms

(22) 2-Butanone (T)

3.990min (+ 0.022) 0.92 ug/L

response 1752

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.30	19.01
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
 Data File : VV020167.D
 Acq On : 25 Jan 2021 22:42
 Operator : SY/MD
 Sample : L5214-05
 Misc : 5.0G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-QT1-2021-01

Manual Integrations
 APPROVED

SAM
 2/1/2021 3:34:36 PM

Quant Time: Jan 26 05:50:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 25 18:17:01 2021
 Response via : Initial Calibration

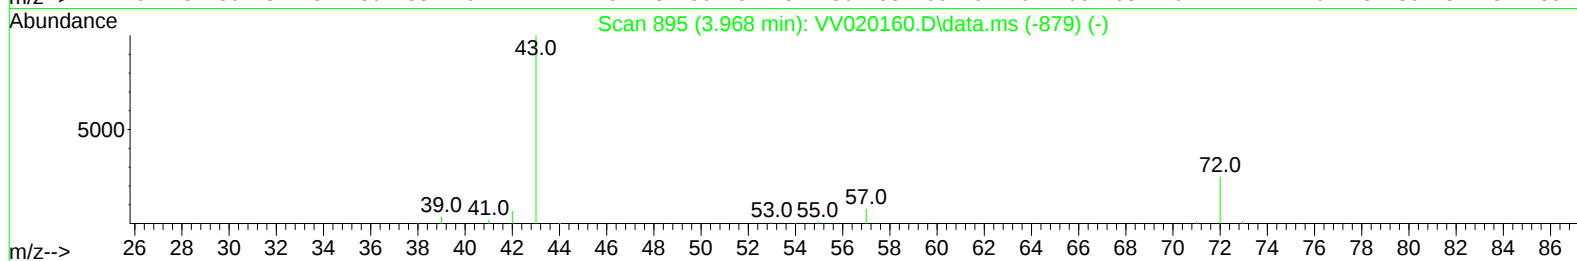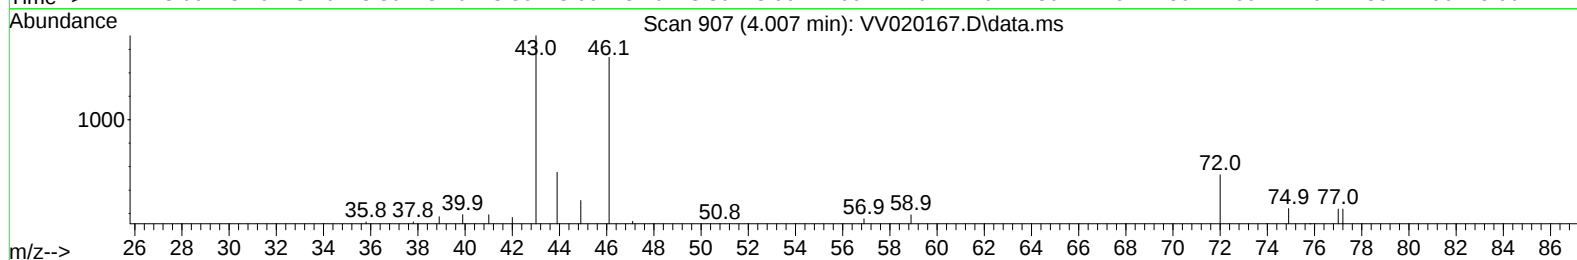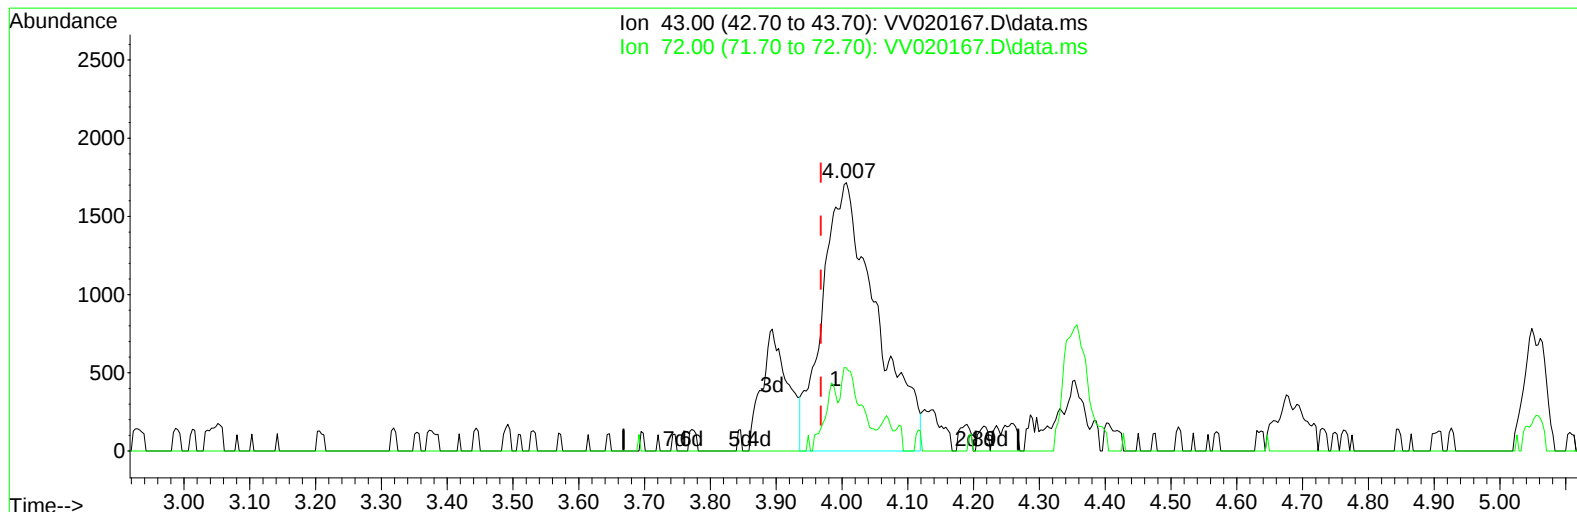

TIC: VV020167.D\data.ms

(22) 2-Butanone (T)

4.007min (+ 0.039) 5.12 ug/L m

response 9713

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.30	3.43#
0.00	0.00	0.00
0.00	0.00	0.00