

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
 Data File : VV020164.D
 Acq On : 25 Jan 2021 21:03
 Operator : SY/MD
 Sample : VV0126MBL01
 Misc : 5.0G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK611

Quant Time: Jan 26 05:49:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 25 18:17:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	417915	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.855	117	394482	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.257	152	180413	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.309	65	183630	55.36	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 110.72%			
7) Chloroethane-d5	1.569	69	141804	56.05	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 112.10%			
11) 1,1-Dichloroethene-d2	2.110	63	256701	43.33	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 86.66%			
21) 2-Butanone-d5	3.888	46	216876	106.45	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 106.45%			
24) Chloroform-d	4.354	84	287587	51.04	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.08%			
26) 1,2-Dichloroethane-d4	5.035	65	209640	55.11	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 110.22%			
32) Benzene-d6	5.055	84	550395	54.39	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 108.78%			
36) 1,2-Dichloropropane-d6	6.074	67	175065	53.01	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 106.02%			
41) Toluene-d8	7.318	98	497399	52.32	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 104.64%			
43) trans-1,3-Dichloroprop...	7.624	79	84554	52.94	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 105.88%			
47) 2-Hexanone-d5	8.090	63	153338	106.92	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 106.92%			
56) 1,1,2,2-Tetrachloroeth...	10.222	84	235648	49.07	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 98.14%			
66) 1,2-Dichlorobenzene-d4	11.633	152	187907	54.76	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 109.52%			
Target Compounds						Qvalue
16) Methylene chloride	2.515	84	882	0.33	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
Data File : VV020164.D
Acq On : 25 Jan 2021 21:03
Operator : SY/MD
Sample : VV0126MBL01
Misc : 5.0G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK611


Quant Time: Jan 26 05:49:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 25 18:17:01 2021
Response via : Initial Calibration

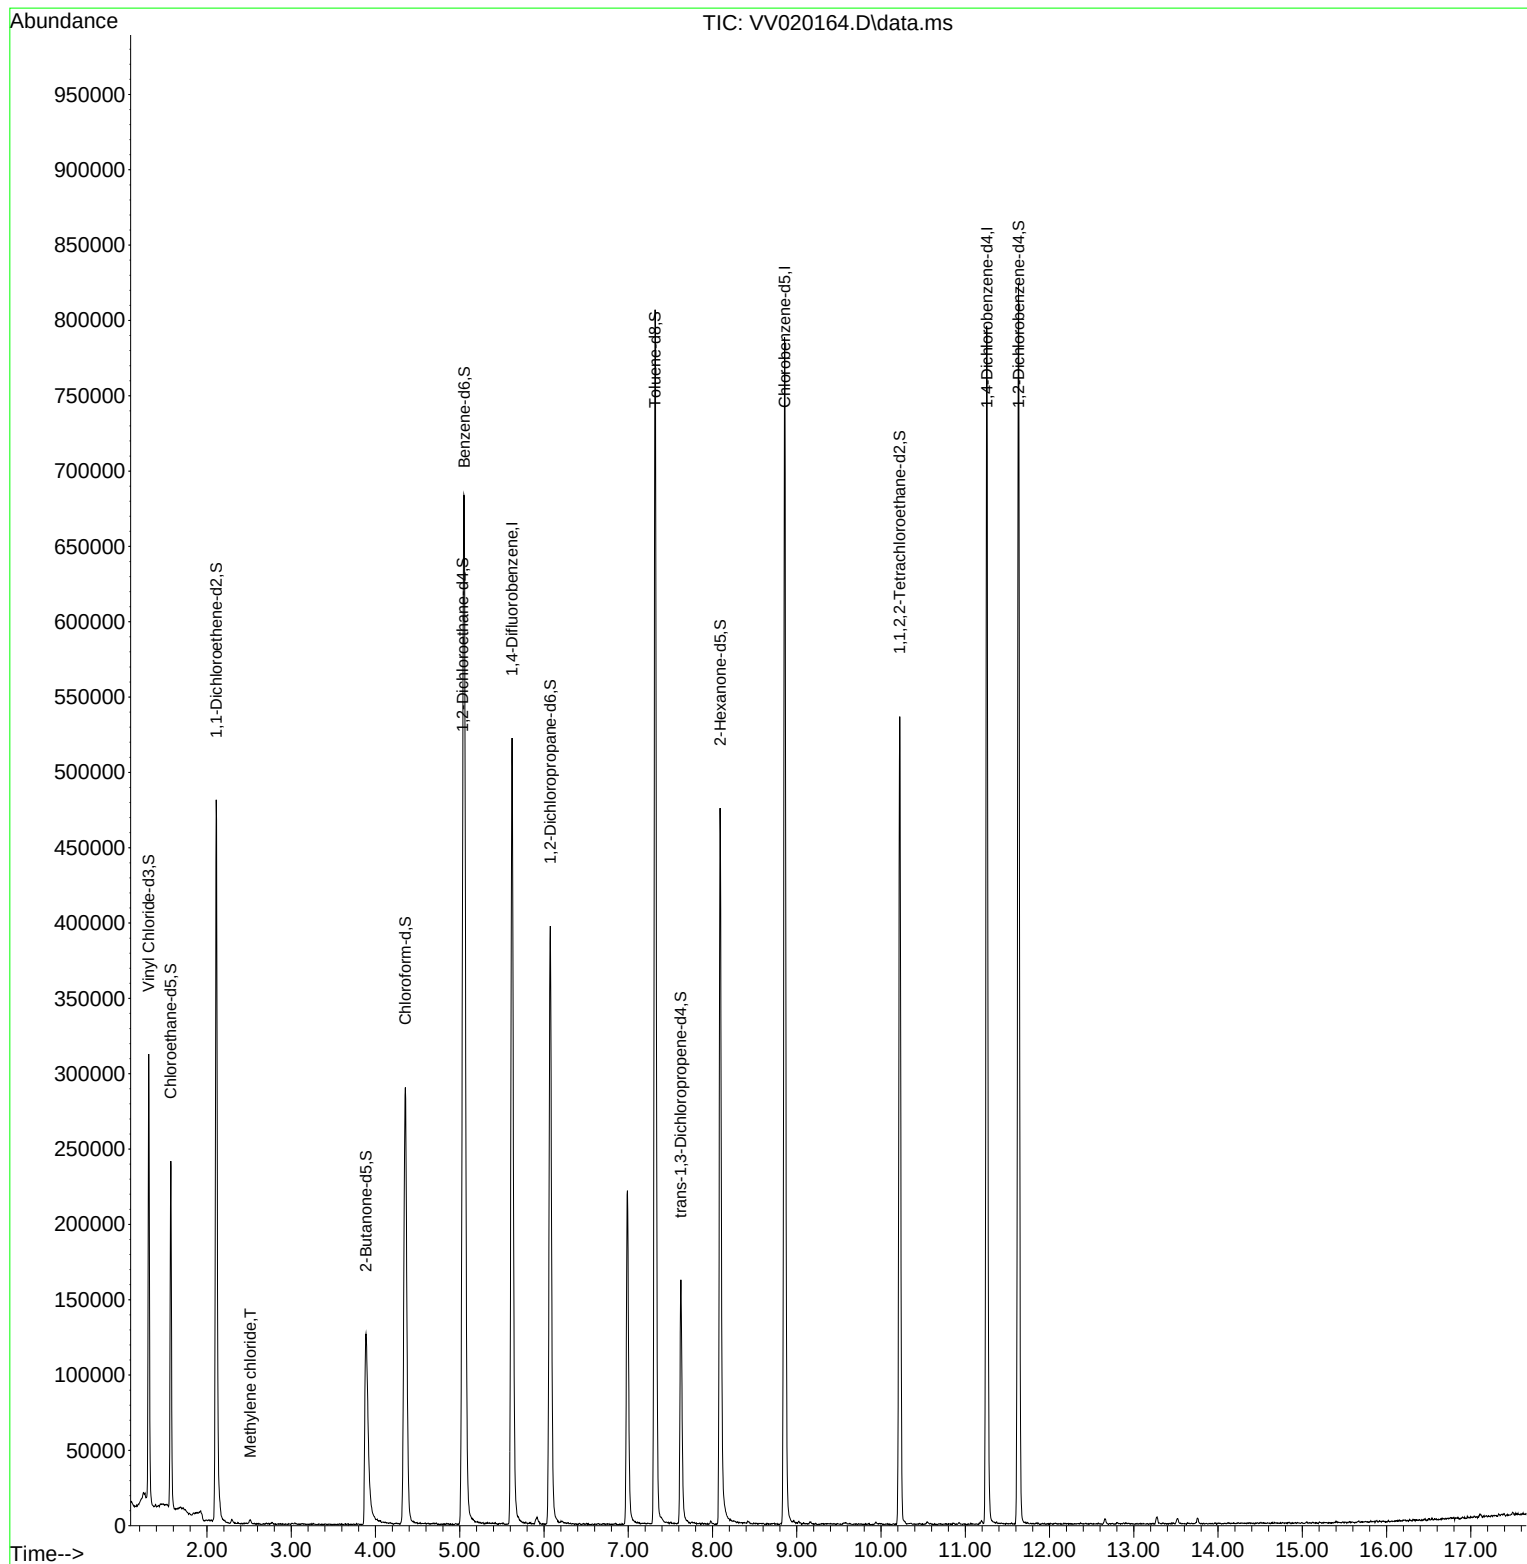

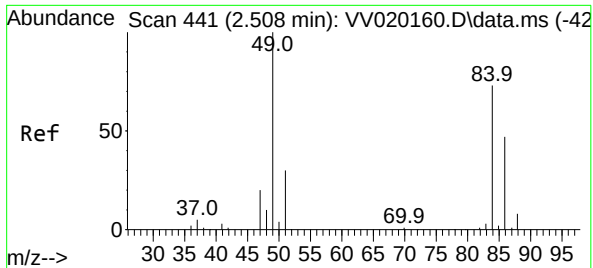

#16
Methylene chloride
Concen: 0.33 ug/L
RT: 2.515 min Scan# 443
Delta R.T. 0.006 min
Lab File: VV020164.D
Acq: 25 Jan 2021 21:03

Instrument :
MSVOA_V
ClientSampleId :
VBLK611

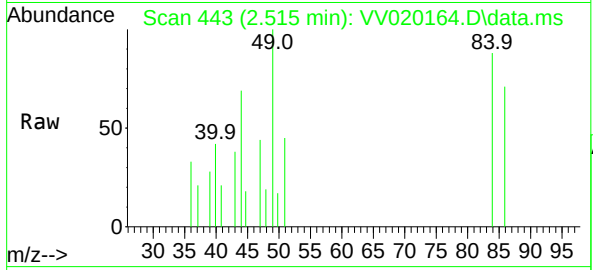

Tgt Ion: 84 Resp: 882

Ion	Ratio	Lower	Upper
84	100		
86	80.0	45.6	84.8
49	113.3	89.3	165.9

