

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
 Data File : VV020165.D
 Acq On : 25 Jan 2021 21:53
 Operator : SY/MD
 Sample : VV0126WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK612

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
 Title : VOC Analysis

Signal : TIC: VV020165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	84	rVB	276682	292583	17.40%	2.171%
2	1.569	143	149	164	rVB	225599	254864	15.16%	1.891%
3	2.109	307	317	344	rVB	446103	671601	39.95%	4.984%
4	2.900	560	563	564	rBV	365	234	0.01%	0.002%
5	3.013	594	598	600	rBV5	1183	746	0.04%	0.006%
6	3.032	602	604	607	rBV2	680	507	0.03%	0.004%
7	3.103	624	626	631	rBV2	595	396	0.02%	0.003%
8	3.257	671	674	677	rBV2	641	446	0.03%	0.003%
9	3.502	747	750	751	rBV	507	260	0.02%	0.002%
10	3.627	787	789	792	rBV3	626	482	0.03%	0.004%
11	3.691	805	809	813	rBV4	567	564	0.03%	0.004%
12	3.714	814	816	818	rVB2	680	258	0.02%	0.002%
13	3.733	818	822	823	rBV2	592	474	0.03%	0.004%
14	3.778	834	836	838	rBV2	449	159	0.01%	0.001%
15	3.888	859	870	902	rBV	124363	359285	21.37%	2.666%
16	4.354	999	1015	1039	rBV	271848	670684	39.89%	4.977%
17	4.614	1093	1096	1097	rBV	511	246	0.01%	0.002%
18	4.666	1110	1112	1113	rBV2	576	172	0.01%	0.001%
19	4.904	1184	1186	1188	rBV3	540	329	0.02%	0.002%
20	4.933	1193	1195	1198	rVB2	657	303	0.02%	0.002%
21	5.048	1213	1231	1259	rBV2	642811	1681254	100.00%	12.476%
22	5.389	1334	1337	1338	rBV2	653	359	0.02%	0.003%
23	5.453	1352	1357	1360	rBV3	1167	956	0.06%	0.007%
24	5.508	1372	1374	1375	rBV	550	154	0.01%	0.001%
25	5.518	1375	1377	1378	rVV2	530	151	0.01%	0.001%
26	5.556	1387	1389	1394	rVB2	547	317	0.02%	0.002%
27	5.621	1396	1409	1433	rBV	517300	1017554	60.52%	7.551%
28	6.074	1536	1550	1574	rBV	382908	778763	46.32%	5.779%
29	6.347	1633	1635	1638	rBV2	236	108	0.01%	0.001%
30	6.363	1638	1640	1642	rVV	553	295	0.02%	0.002%
31	6.389	1646	1648	1649	rBV	263	74	0.00%	0.001%
32	6.421	1656	1658	1660	rBV2	528	312	0.02%	0.002%
33	6.576	1704	1706	1710	rBV5	505	274	0.02%	0.002%
34	6.601	1712	1714	1719	rVB4	649	365	0.02%	0.003%
35	6.627	1719	1722	1723	rBV	884	448	0.03%	0.003%
36	6.813	1778	1780	1782	rVB2	572	225	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
 Data File : VV020165.D
 Acq On : 25 Jan 2021 21:53
 Operator : SY/MD
 Sample : VV0126WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK612

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
 Title : VOC Analysis

37	6.842	1785	1789	1790	rBV3	467	314	0.02%	0.002%
38	6.907	1806	1809	1811	rBV3	803	610	0.04%	0.005%
39	6.990	1821	1835	1857	rBV	207848	373985	22.24%	2.775%
40	7.318	1925	1937	1959	rBV	751039	1281701	76.23%	9.511%
41	7.624	2022	2032	2060	rBV	164326	283990	16.89%	2.107%
42	7.801	2084	2087	2089	rBV2	689	305	0.02%	0.002%
43	7.878	2110	2111	2113	rVB2	201	75	0.00%	0.001%
44	7.916	2118	2123	2127	rBV2	418	429	0.03%	0.003%
45	7.987	2136	2145	2151	rBV5	1893	2343	0.14%	0.017%
46	8.090	2167	2177	2209	rBV	547285	910142	54.13%	6.754%
47	8.415	2274	2278	2279	rBV3	1993	1432	0.09%	0.011%
48	8.572	2325	2327	2330	rBV2	606	320	0.02%	0.002%
49	8.704	2365	2368	2371	rBV2	512	292	0.02%	0.002%
50	8.801	2397	2398	2399	rBV	522	148	0.01%	0.001%
51	8.855	2403	2415	2435	rBV	898537	1434177	85.30%	10.643%
52	9.206	2522	2524	2527	rVB2	703	338	0.02%	0.003%
53	9.283	2544	2548	2551	rVB4	991	577	0.03%	0.004%
54	9.302	2551	2554	2557	rBV4	963	762	0.05%	0.006%
55	9.444	2595	2598	2600	rBV4	441	259	0.02%	0.002%
56	9.865	2726	2729	2733	rBV3	563	465	0.03%	0.003%
57	9.929	2746	2749	2750	rBV	683	398	0.02%	0.003%
58	10.157	2819	2820	2821	rBV	442	110	0.01%	0.001%
59	10.222	2828	2840	2857	rBV	521929	812018	48.30%	6.026%
60	10.518	2931	2932	2935	rVB2	791	276	0.02%	0.002%
61	10.534	2935	2937	2939	rBV3	574	284	0.02%	0.002%
62	10.665	2976	2978	2979	rBV	485	155	0.01%	0.001%
63	10.781	3011	3014	3015	rBV2	450	236	0.01%	0.002%
64	10.826	3024	3028	3032	rBV4	632	543	0.03%	0.004%
65	11.116	3114	3118	3121	rBV5	672	656	0.04%	0.005%
66	11.164	3131	3133	3136	rBV2	682	400	0.02%	0.003%
67	11.257	3150	3162	3186	rBV	848132	1259087	74.89%	9.343%
68	11.630	3266	3278	3301	rBV	874893	1361504	80.98%	10.103%
69	11.955	3375	3379	3380	rBV	173	134	0.01%	0.001%
70	12.083	3412	3419	3425	rBV3	360	510	0.03%	0.004%
71	12.157	3435	3442	3445	rBV2	410	449	0.03%	0.003%
72	12.353	3500	3503	3505	rBV	304	191	0.01%	0.001%
73	12.392	3512	3515	3518	rBV	214	191	0.01%	0.001%
74	12.463	3535	3537	3540	rBV	267	220	0.01%	0.002%
75	12.514	3552	3553	3554	rBV	123	33	0.00%	0.000%
76	12.546	3559	3563	3565	rBV	267	176	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
 Data File : VV020165.D
 Acq On : 25 Jan 2021 21:53
 Operator : SY/MD
 Sample : VV0126WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK612

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M

Title : VOC Analysis

77	12.659	3593	3598	3603	rVB5	1755	1890	0.11%	0.014%
78	12.842	3654	3655	3657	rBV	218	68	0.00%	0.001%
79	12.910	3674	3676	3677	rBV	203	73	0.00%	0.001%
80	12.980	3696	3698	3702	rVB2	393	177	0.01%	0.001%
81	13.103	3734	3736	3738	rBV2	245	123	0.01%	0.001%
82	13.241	3777	3779	3783	rBV2	244	167	0.01%	0.001%
83	13.276	3783	3790	3798	rBV6	1988	3113	0.19%	0.023%
84	13.427	3834	3837	3839	rBV2	547	314	0.02%	0.002%
85	13.447	3839	3843	3844	rBV	489	331	0.02%	0.002%
86	13.524	3859	3867	3875	rBV4	1591	2439	0.15%	0.018%
87	13.601	3887	3891	3892	rBV	222	154	0.01%	0.001%
88	13.627	3896	3899	3901	rBV2	461	304	0.02%	0.002%




Sum of corrected areas: 13475590

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
Data File : VV020165.D
Acq On : 25 Jan 2021 21:53
Operator : SY/MD
Sample : VV0126WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

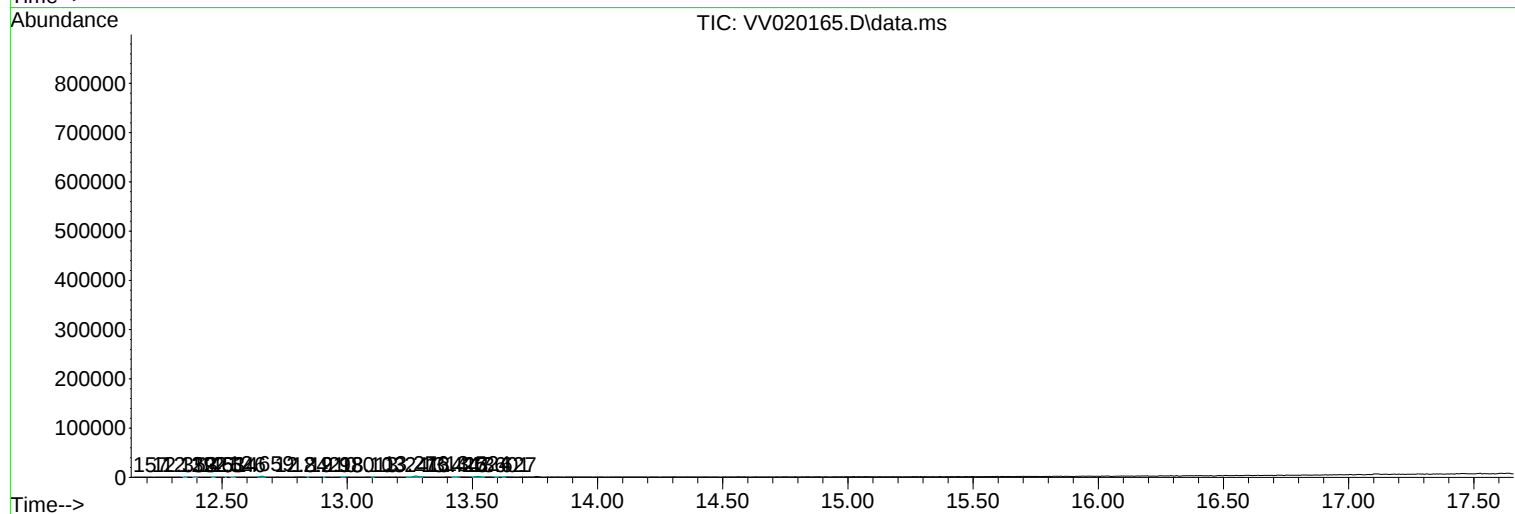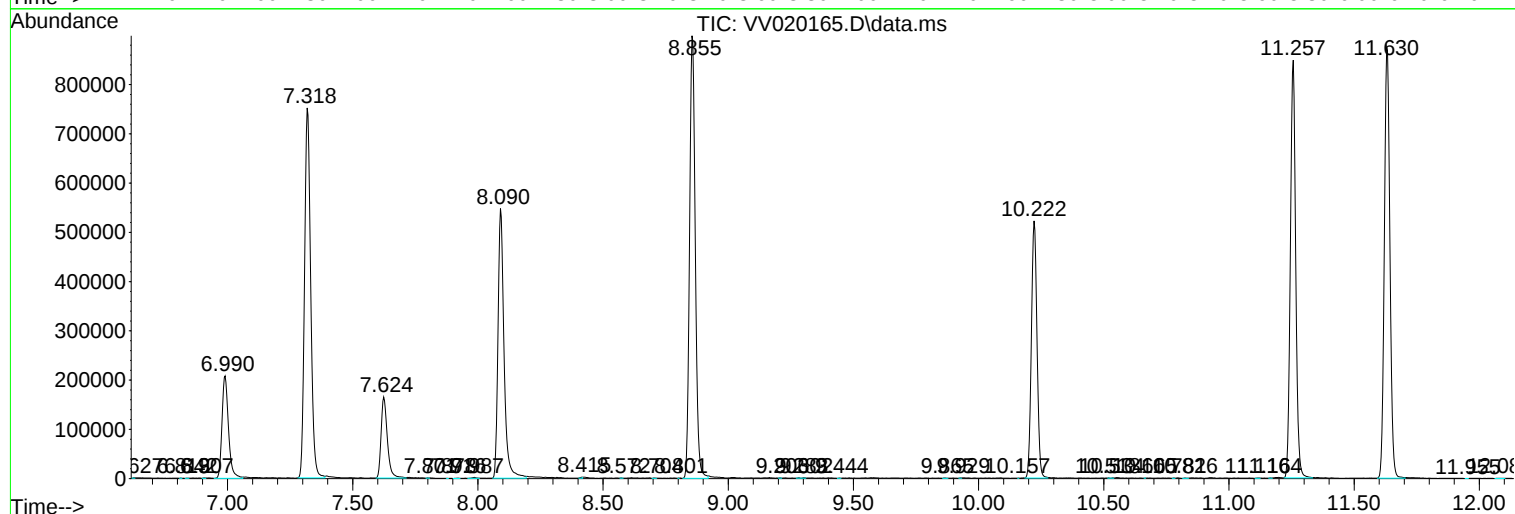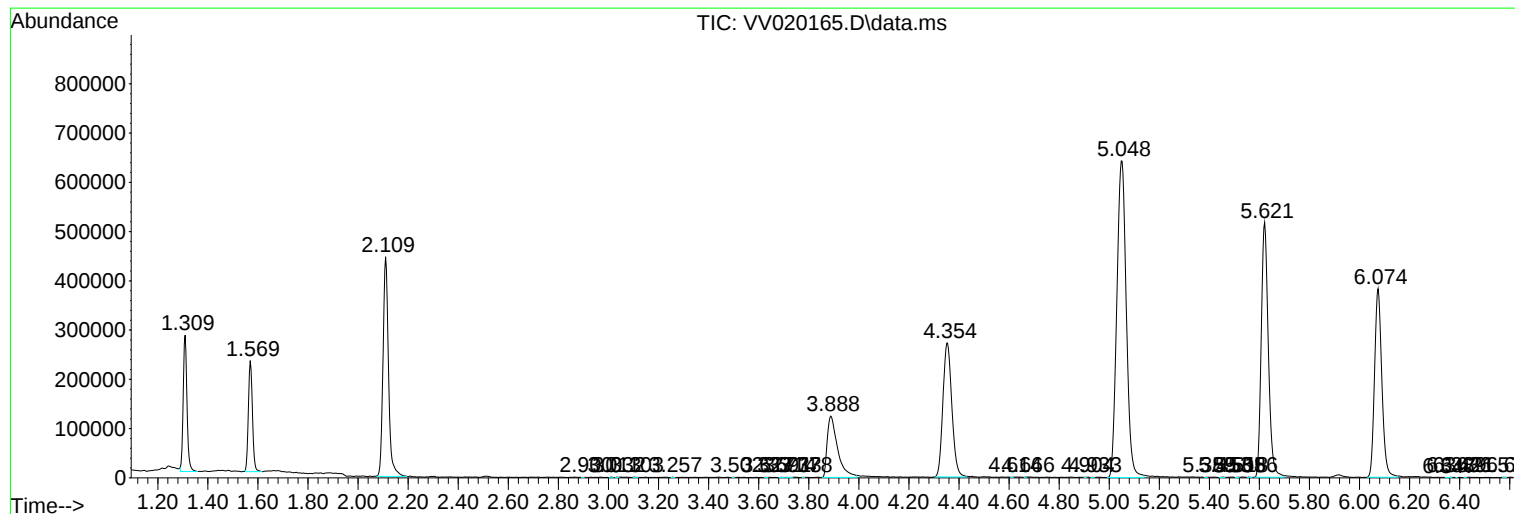

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
Data File : VV020165.D
Acq On : 25 Jan 2021 21:53
Operator : SY/MD
Sample : VV0126WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
Data File : VV020165.D
Acq On : 25 Jan 2021 21:53
Operator : SY/MD
Sample : VV0126WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
