
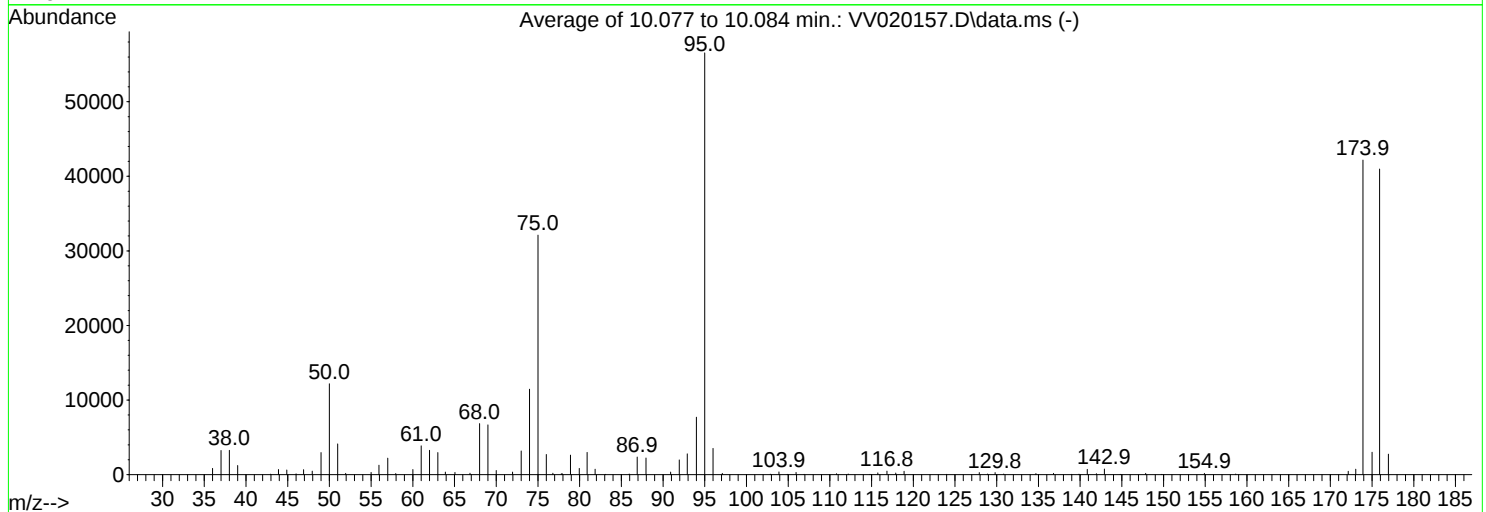


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012621\
 Data File : VV020157.D
 Acq On : 25 Jan 2021 15:07
 Operator : SY/MD
 Sample : BFB81
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB811

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM012621WMA.M
 Title : VOC Analysis
 Last Update : Wed Jan 27 06:32:48 2021

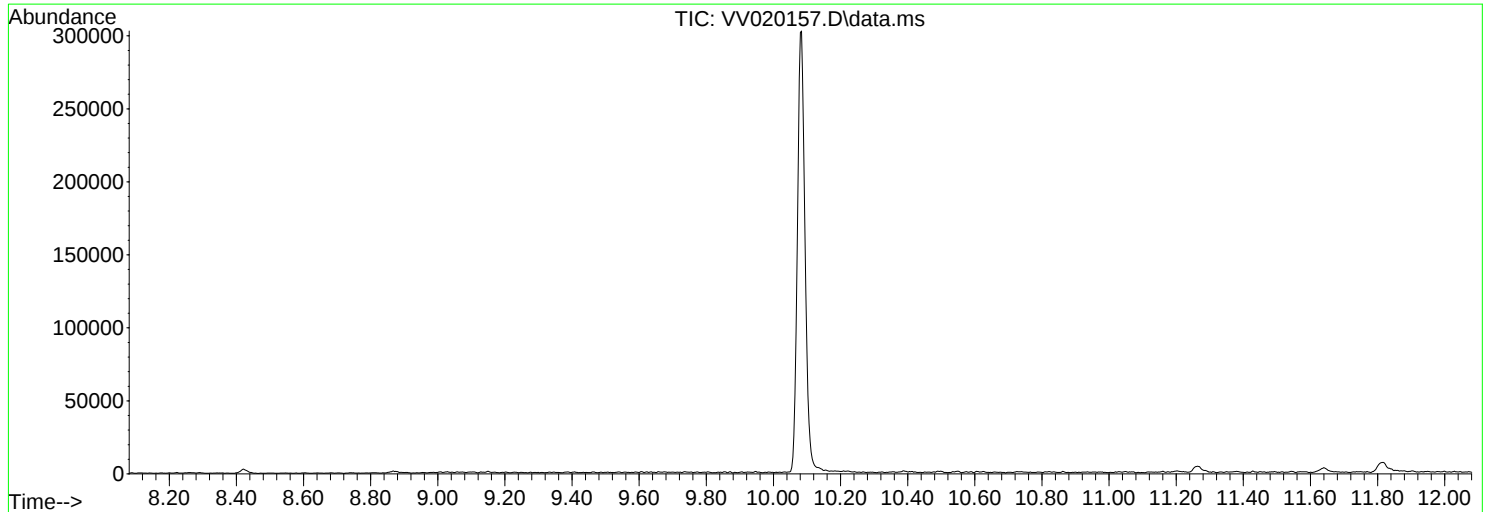

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	12186	PASS
75	95	30	80	56.8	32123	PASS
95	95	100	100	100.0	56552	PASS
96	95	5	9	6.2	3512	PASS
173	174	0.00	2	1.7	730	PASS
174	95	50	120	74.6	42176	PASS
175	174	5	9	7.1	3011	PASS
176	174	95	101	97.2	40984	PASS
177	176	5	9	6.7	2739	PASS

m/z	Abundance
37.30	124.0
38.30	182.0
39.10	144.0
39.80	211.0
41.30	113.0
42.90	100.0
43.90	426.0

Instrument :
MSVOA_V
ClientSampleId :
BFB811

m/z	Abundance
36.00	785.0
37.00	3192.0
38.00	2925.0
39.00	1283.0
39.90	222.0
43.00	148.0
43.90	1178.0
44.90	552.0
46.00	113.0
46.90	626.0
47.90	434.0
49.00	2624.0
50.00	11842.0
51.00	3984.0
51.90	193.0
55.00	221.0
55.90	1200.0
57.00	2129.0
57.90	186.0
60.00	715.0
61.00	3684.0
62.00	2982.0
63.00	2759.0
63.90	283.0
65.00	230.0
66.80	161.0
68.00	6470.0
69.00	6324.0
70.00	449.0
72.00	354.0
73.00	3121.0
74.00	10641.0
75.00	29744.0
76.00	2733.0
76.80	272.0
77.80	202.0
78.00	174.0
78.90	2500.0
80.00	813.0
80.90	2842.0
81.90	634.0
86.90	2188.0
87.90	1999.0
90.90	347.0
92.00	1751.0
92.90	2611.0
94.00	7269.0
95.00	53000.0
96.00	3342.0
97.10	184.0
102.80	109.0
103.90	296.0
106.00	284.0
110.80	121.0
115.70	217.0
116.80	394.0
117.90	194.0
118.90	343.0
124.00	108.0
127.90	232.0
129.80	236.0
134.70	145.0
136.80	169.0
139.00	112.0
140.90	680.0
142.00	129.0
142.90	610.0
144.80	121.0
147.80	142.0
154.90	167.0
172.20	367.0
173.00	665.0
173.90	38392.0
175.00	2746.0
175.90	36640.0
177.00	2643.0

Instrument :
MSVOA_V
ClientSampleId :
BFB811

m/z	Abundance
36.00	856.0
37.00	3375.0
38.00	3397.0
39.00	1401.0
39.90	198.0
43.00	171.0
43.90	1137.0
44.90	657.0
46.00	105.0
46.90	713.0
47.90	488.0
49.00	3079.0
50.00	12570.0
51.00	4273.0
51.90	180.0
55.00	303.0
56.00	1306.0
57.00	2335.0
58.00	163.0
60.00	705.0
61.00	3993.0
62.00	3339.0
63.00	3077.0
63.90	352.0
65.10	314.0
66.90	204.0
68.00	7138.0
69.00	6873.0
70.00	573.0
71.90	375.0
73.00	3307.0
74.00	11944.0
75.00	33400.0
76.00	2811.0
77.80	180.0
78.90	2693.0
79.90	865.0
80.90	3140.0
81.80	786.0
85.90	103.0
86.90	2482.0
88.00	2305.0
90.90	352.0
91.90	2077.0
92.90	2964.0
94.00	7989.0
95.00	58424.0
96.00	3663.0
97.10	167.0
102.90	110.0
103.90	399.0
104.90	102.0
105.90	312.0
110.80	156.0
112.20	124.0
115.80	235.0
116.90	472.0
117.90	212.0
118.90	462.0
127.90	300.0
128.90	136.0
129.80	298.0
130.90	129.0
134.70	161.0
136.80	181.0
139.90	106.0
140.80	702.0
142.00	140.0
142.90	768.0
147.90	163.0
154.90	185.0
158.70	134.0
172.10	461.0
173.00	749.0
173.90	43640.0
175.00	3017.0
175.90	42416.0
177.00	2808.0

Instrument :
MSVOA_V
ClientSampleId :
BFB811

m/z	Abundance
36.00	856.0
37.00	3187.0
38.00	3466.0
39.00	1393.0
39.90	201.0
43.10	154.0
43.90	1012.0
44.90	682.0
46.00	114.0
46.90	657.0
48.00	472.0
49.00	3178.0
50.00	12147.0
51.00	4126.0
52.00	177.0
55.00	354.0
56.00	1286.0
57.00	2150.0
58.00	113.0
60.00	651.0
61.00	3935.0
62.00	3469.0
63.00	3025.0
63.90	382.0
65.10	366.0
66.90	245.0
68.00	6950.0
69.00	6819.0
70.00	652.0
71.90	334.0
73.00	3086.0
74.00	11803.0
75.00	33224.0
76.00	2577.0
76.80	323.0
77.90	174.0
78.90	2671.0
79.90	840.0
80.90	2969.0
81.80	795.0
83.10	129.0
86.00	162.0
86.90	2391.0
88.00	2396.0
90.90	339.0
91.90	2079.0
92.90	2828.0
94.00	7860.0
95.00	58232.0
96.00	3530.0
97.10	149.0
103.90	430.0
105.90	303.0
106.90	112.0
110.80	126.0
112.20	115.0
114.80	109.0
115.80	261.0
116.90	561.0
117.90	241.0
118.90	562.0
127.90	283.0
128.90	130.0
129.80	317.0
130.80	147.0
134.70	152.0
136.80	175.0
139.80	111.0
140.80	715.0
141.90	132.0
142.90	893.0
147.90	183.0
149.80	126.0
154.90	165.0
158.60	120.0
172.10	545.0
173.10	777.0
173.90	44496.0
175.00	3270.0
175.90	43896.0
176.90	2766.0

Instrument :
MSVOA_V
ClientSampleId :
BFB811