

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012622\
 Data File : VW024433.D
 Acq On : 26 Jan 2022 12:54
 Operator : SY/MD
 Sample : VW0126WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK296

Quant Time: Jan 27 03:49:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 27 01:56:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	170917	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	185102	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	91866	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	76821	5.130	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.600%
7) Chloroethane-d5	1.568	69	67327	5.154	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.000%
11) 1,1-Dichloroethene-d2	2.108	63	116833	4.082	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.600%
20) 2-Butanone-d5	3.928	46	104946	43.975	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.960%
24) Chloroform-d	4.352	84	143382	5.046	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.000%
26) 1,2-Dichloroethane-d4	5.034	65	68050	5.288	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.800%
32) Benzene-d6	5.050	84	277717	5.024	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
36) 1,2-Dichloropropane-d6	6.072	67	88640	5.092	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.800%
41) Toluene-d8	7.317	98	238100	4.694	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.800%
43) trans-1,3-Dichloroprop...	7.625	79	28446	4.759	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.200%
46) 2-Hexanone-d5	8.091	63	92392	45.202	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.400%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	48582	4.689	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	87969	5.584	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.600%
Target Compounds						
25) Chloroform	4.371	83	5790	0.222	ug/L	Qvalue 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024433.D
Acq On : 26 Jan 2022 12:54
Operator : SY/MD
Sample : VV0126WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK296

Quant Time: Jan 27 03:49:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 27 01:56:16 2022
Response via : Initial Calibration

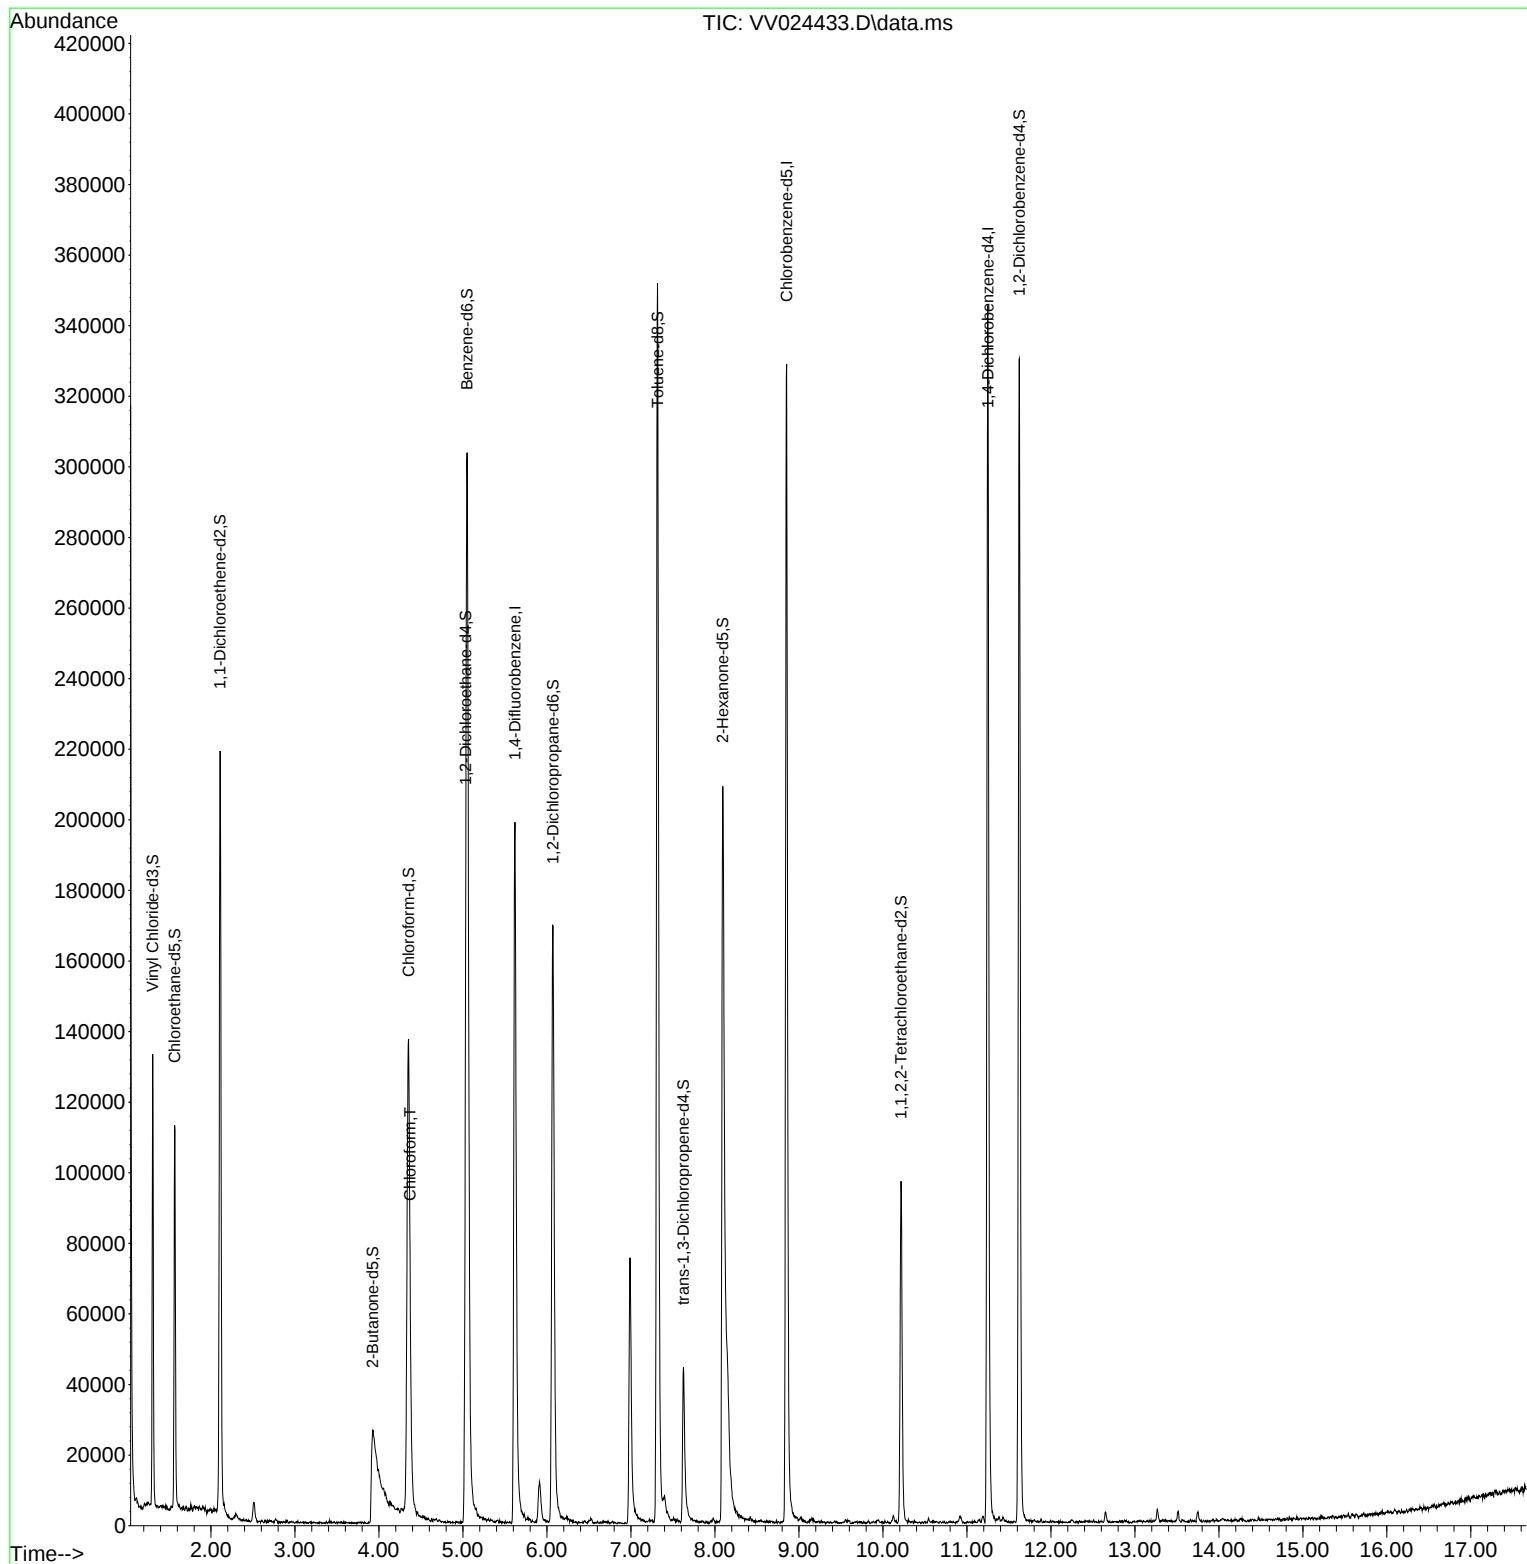

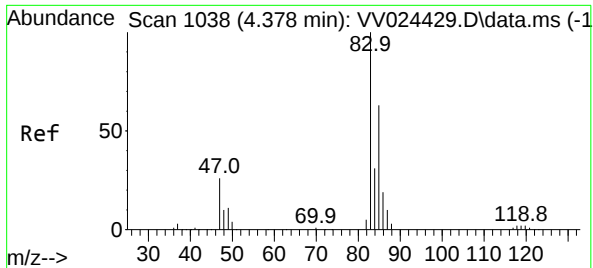

#25
 Chloroform
 Concen: 0.222 ug/L
 RT: 4.371 min Scan# 10
 Delta R.T. -0.007 min
 Lab File: VV024433.D
 Acq: 26 Jan 2022 12:54

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK296

Tgt Ion: 83 Resp: 5790
 Ion Ratio Lower Upper
 83 100
 85 79.1 45.2 84.0

