

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012622\
 Data File : VW024435.D
 Acq On : 26 Jan 2022 13:41
 Operator : SY/MD
 Sample : N1275-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F24

Quant Time: Jan 27 03:50:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 27 01:56:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	167869	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	177174	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	88090	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	72649	4.940	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.800%
7) Chloroethane-d5	1.568	69	67123	5.232	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.600%
11) 1,1-Dichloroethene-d2	2.108	63	111649	3.972	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.400%
20) 2-Butanone-d5	3.921	46	76520	32.646	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	65.300%
24) Chloroform-d	4.352	84	138101	4.949	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
26) 1,2-Dichloroethane-d4	5.034	65	65754	5.202	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.000%
32) Benzene-d6	5.050	84	261850	4.949	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
36) 1,2-Dichloropropane-d6	6.069	67	83123	4.989	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.800%
41) Toluene-d8	7.317	98	223683	4.607	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.200%
43) trans-1,3-Dichloroprop...	7.625	79	26511	4.633	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.600%
46) 2-Hexanone-d5	8.091	63	91091	46.560	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.120%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	48711	4.912	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	82911	5.489	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.800%
Target Compounds					Qvalue	
25) Chloroform	4.378	83	6756	0.264	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024435.D
Acq On : 26 Jan 2022 13:41
Operator : SY/MD
Sample : N1275-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F24

Quant Time: Jan 27 03:50:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 27 01:56:16 2022
Response via : Initial Calibration

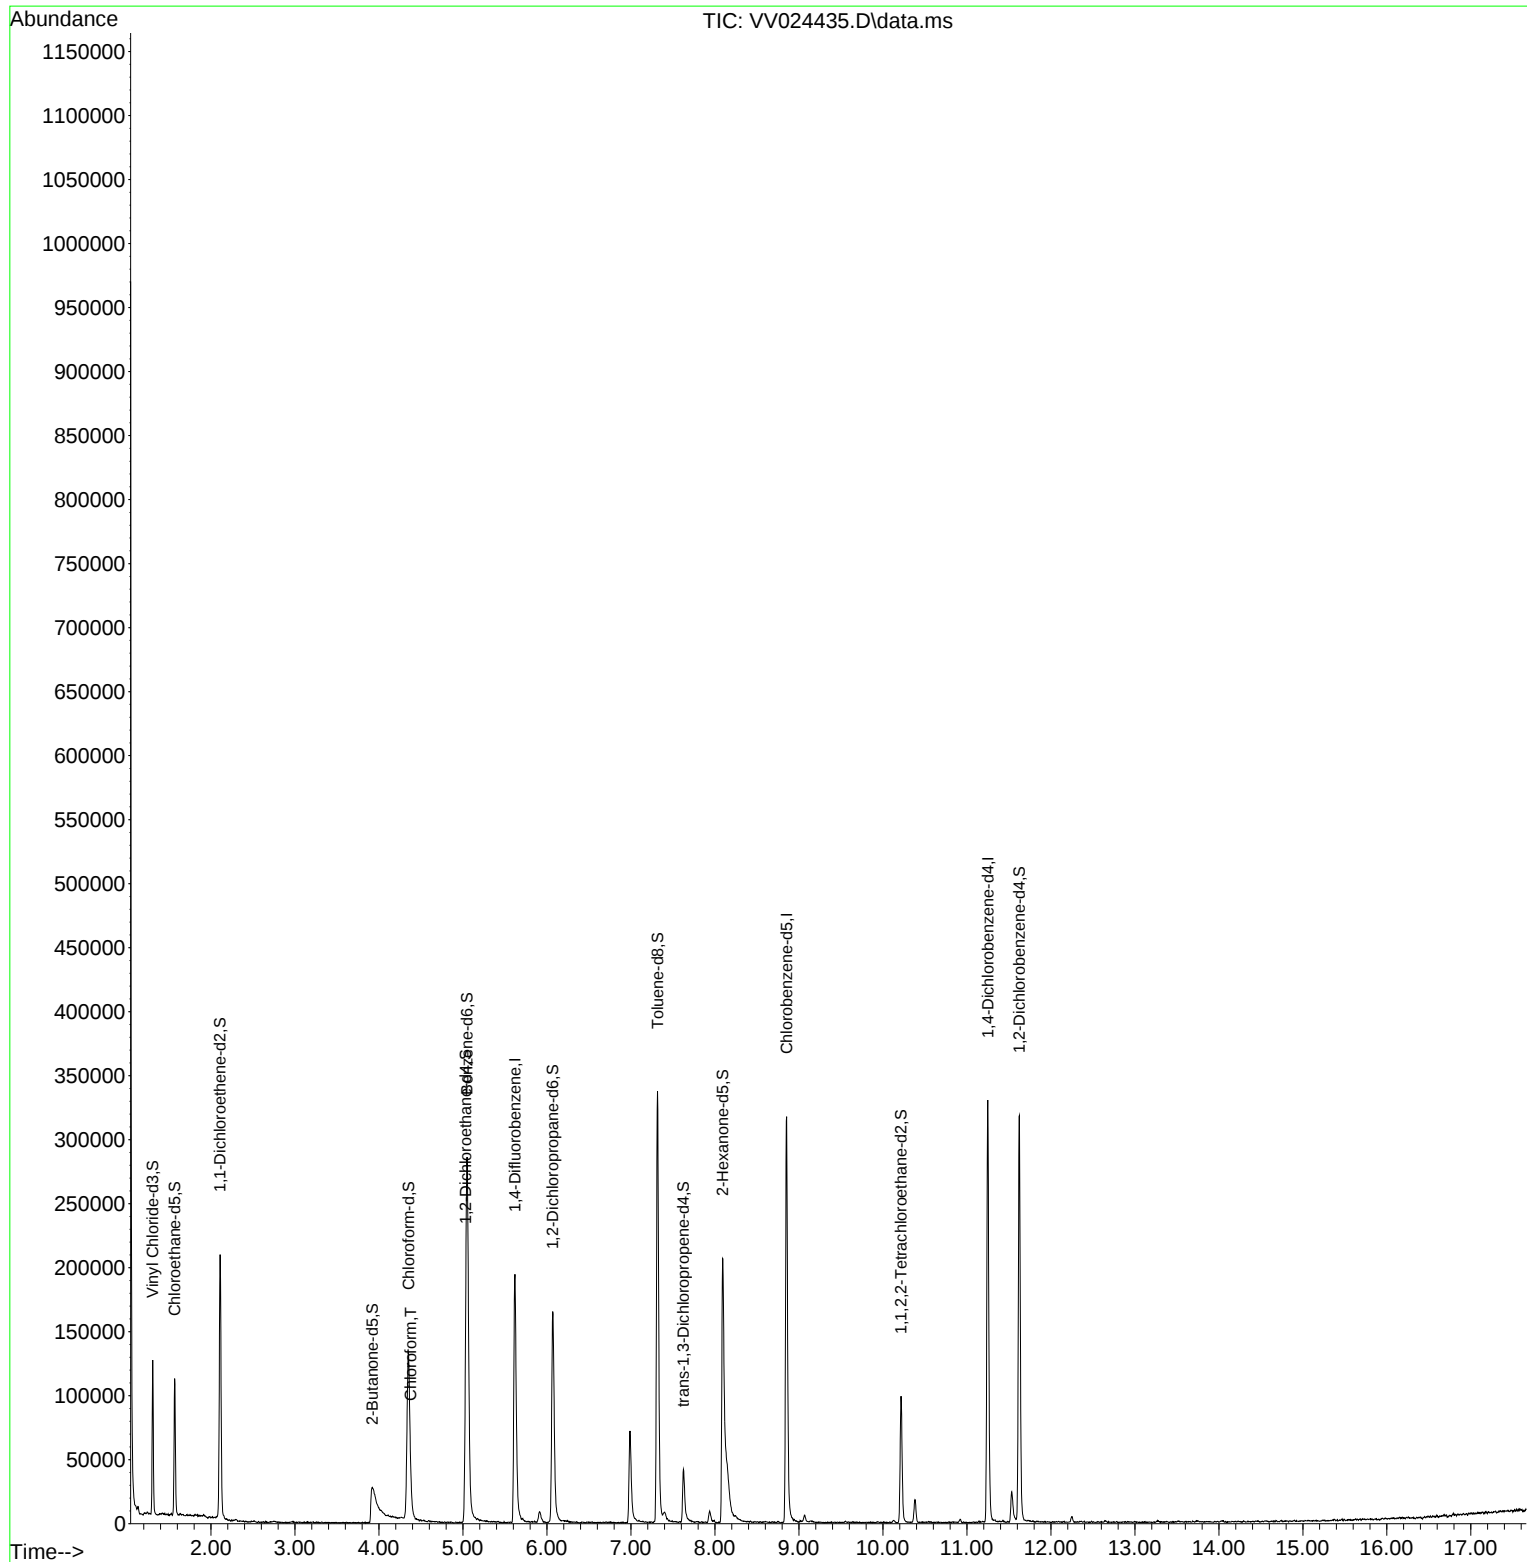

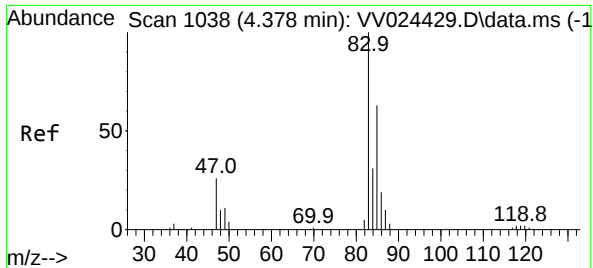

#25
 Chloroform
 Concen: 0.264 ug/L
 RT: 4.378 min Scan# 10
 Delta R.T. -0.000 min
 Lab File: VV024435.D
 Acq: 26 Jan 2022 13:41

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F24

Tgt Ion: 83 Resp: 6756
 Ion Ratio Lower Upper
 83 100
 85 76.5 45.2 84.0

