

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012622\
 Data File : VW024438.D
 Acq On : 26 Jan 2022 14:51
 Operator : SY/MD
 Sample : N1275-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F27

Quant Time: Jan 27 03:50:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 27 01:56:16 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	152119	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	162614	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	78356	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	70299	5.275	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 105.400%		
7) Chloroethane-d5	1.571	69	68957	5.932	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 118.600%		
11) 1,1-Dichloroethene-d2	2.111	63	110624	4.343	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 86.800%		
20) 2-Butanone-d5	3.915	46	135839	63.954	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 127.900%		
24) Chloroform-d	4.352	84	133641	5.285	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 105.600%		
26) 1,2-Dichloroethane-d4	5.037	65	64796	5.657	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 113.200%		
32) Benzene-d6	5.053	84	251288	5.174	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 103.400%		
36) 1,2-Dichloropropane-d6	6.069	67	84439	5.521	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 110.400%		
41) Toluene-d8	7.317	98	212687	4.773	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 95.400%		
43) trans-1,3-Dichloroprop...	7.625	79	25517	4.859	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 97.200%		
46) 2-Hexanone-d5	8.091	63	91257	50.821	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 101.640%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	47718	5.242	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 104.800%		
66) 1,2-Dichlorobenzene-d4	11.625	152	73549	5.474	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 109.400%		
Target Compounds						
25) Chloroform	4.384	83	9109	0.392	ug/L	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024438.D
Acq On : 26 Jan 2022 14:51
Operator : SY/MD
Sample : N1275-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F27

Quant Time: Jan 27 03:50:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 27 01:56:16 2022
Response via : Initial Calibration

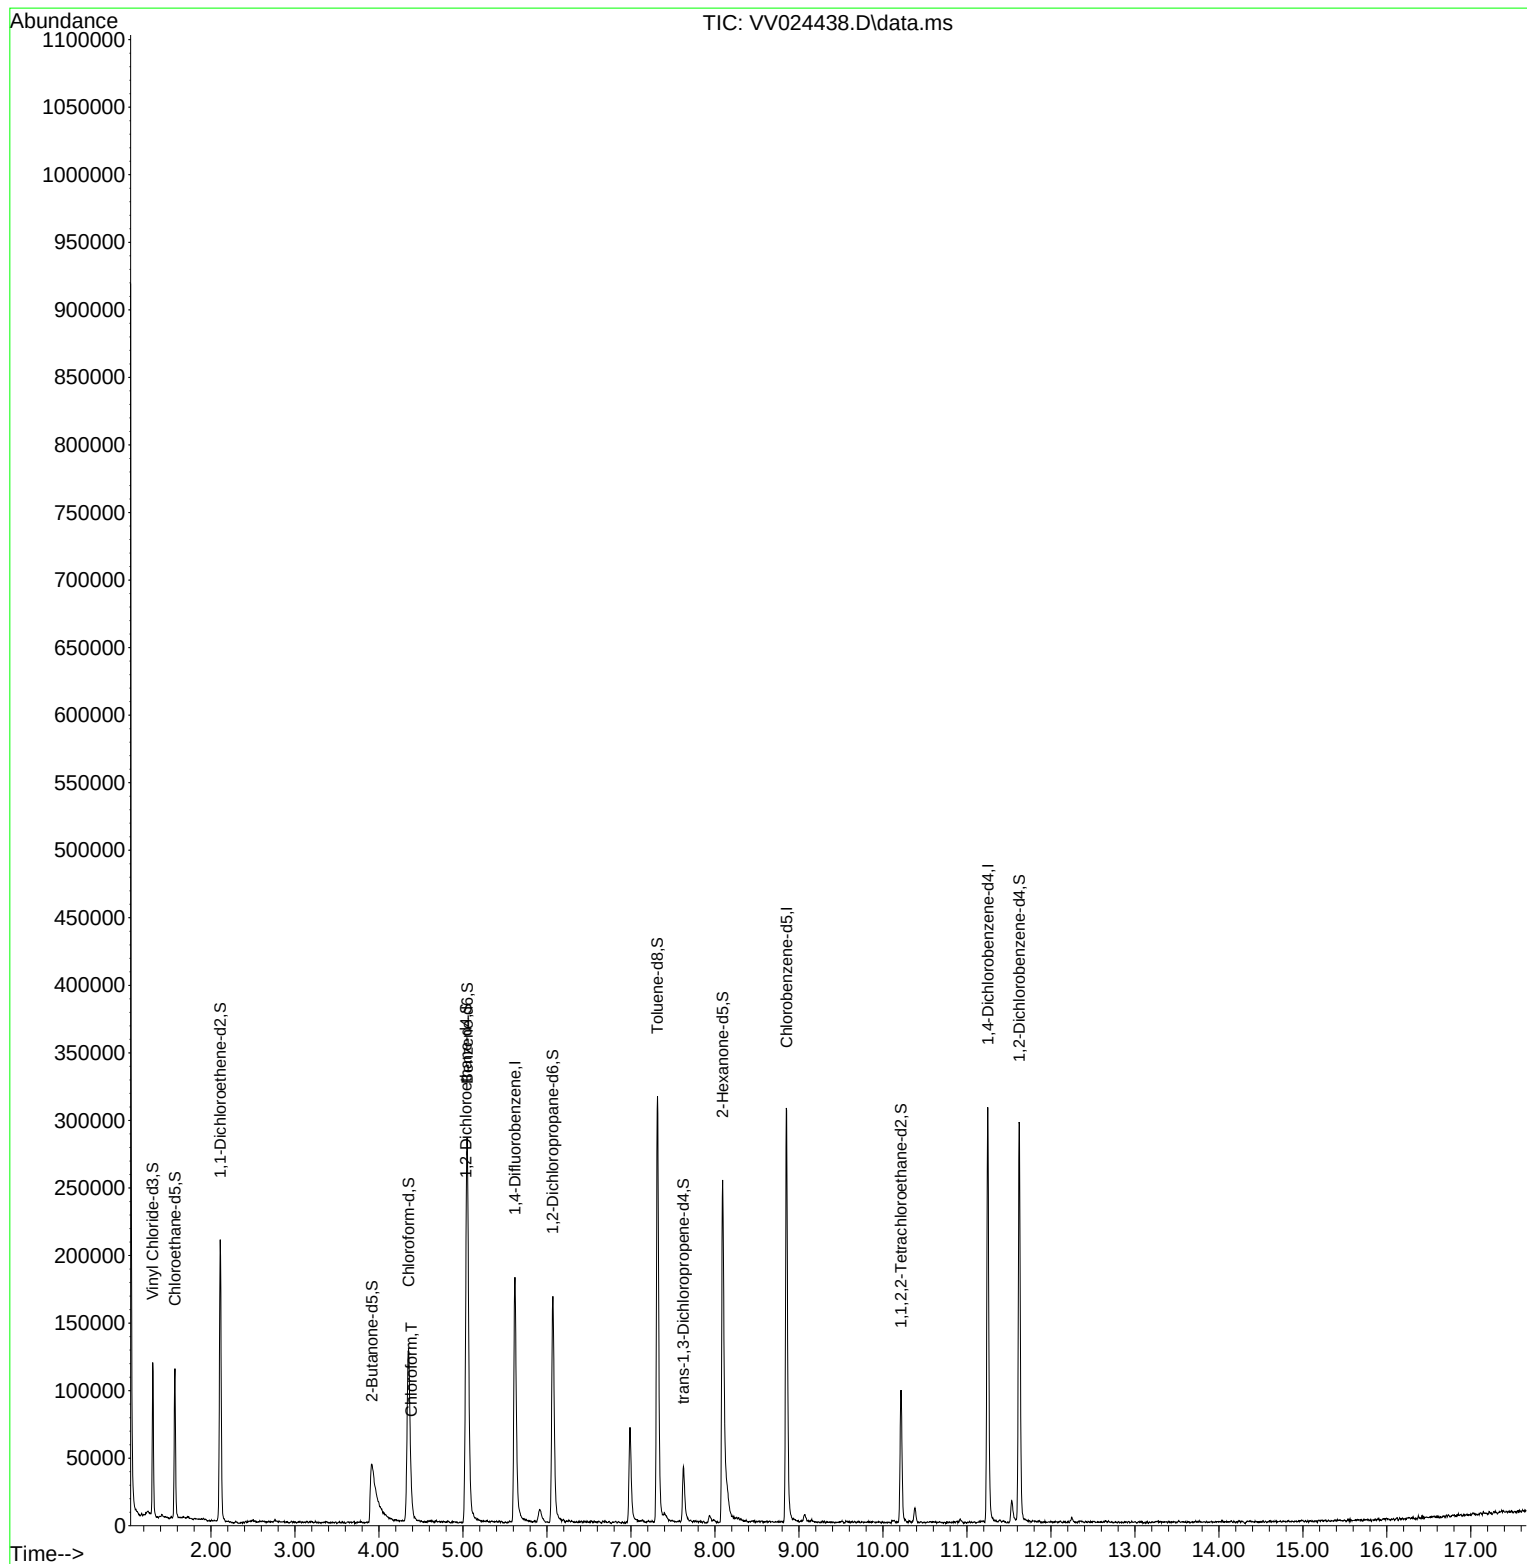

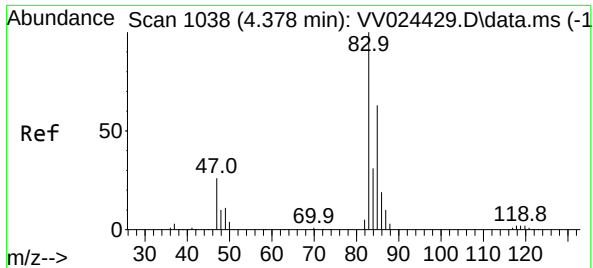

#25
 Chloroform
 Concen: 0.392 ug/L
 RT: 4.384 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: VV024438.D
 Acq: 26 Jan 2022 14:51

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F27

Tgt Ion: 83 Resp: 9109
 Ion Ratio Lower Upper
 83 100
 85 52.1 45.2 84.0

