

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012622\
 Data File : VW024439.D
 Acq On : 26 Jan 2022 15:14
 Operator : SY/MD
 Sample : N1275-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F28

Quant Time: Jan 27 03:50:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 27 01:56:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	143800	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	157121	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73464	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	70759	5.617	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	112.400%
7) Chloroethane-d5	1.568	69	67836	6.173	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	123.400%
11) 1,1-Dichloroethene-d2	2.111	63	110972	4.608	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	92.200%
20) 2-Butanone-d5	3.915	46	93677	46.655	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.320%
24) Chloroform-d	4.352	84	136340	5.703	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.000%
26) 1,2-Dichloroethane-d4	5.037	65	65500	6.050	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	121.000%
32) Benzene-d6	5.050	84	255027	5.435	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.600%
36) 1,2-Dichloropropane-d6	6.069	67	85021	5.754	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	115.000%
41) Toluene-d8	7.317	98	210461	4.888	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.800%
43) trans-1,3-Dichloroprop...	7.625	79	25645	5.054	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.000%
46) 2-Hexanone-d5	8.092	63	92492	53.310	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.620%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	48698	5.537	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	74330	5.900	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.000%
Target Compounds					Qvalue	
25) Chloroform	4.381	83	5360	0.244	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024439.D
Acq On : 26 Jan 2022 15:14
Operator : SY/MD
Sample : N1275-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F28

Quant Time: Jan 27 03:50:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 27 01:56:16 2022
Response via : Initial Calibration

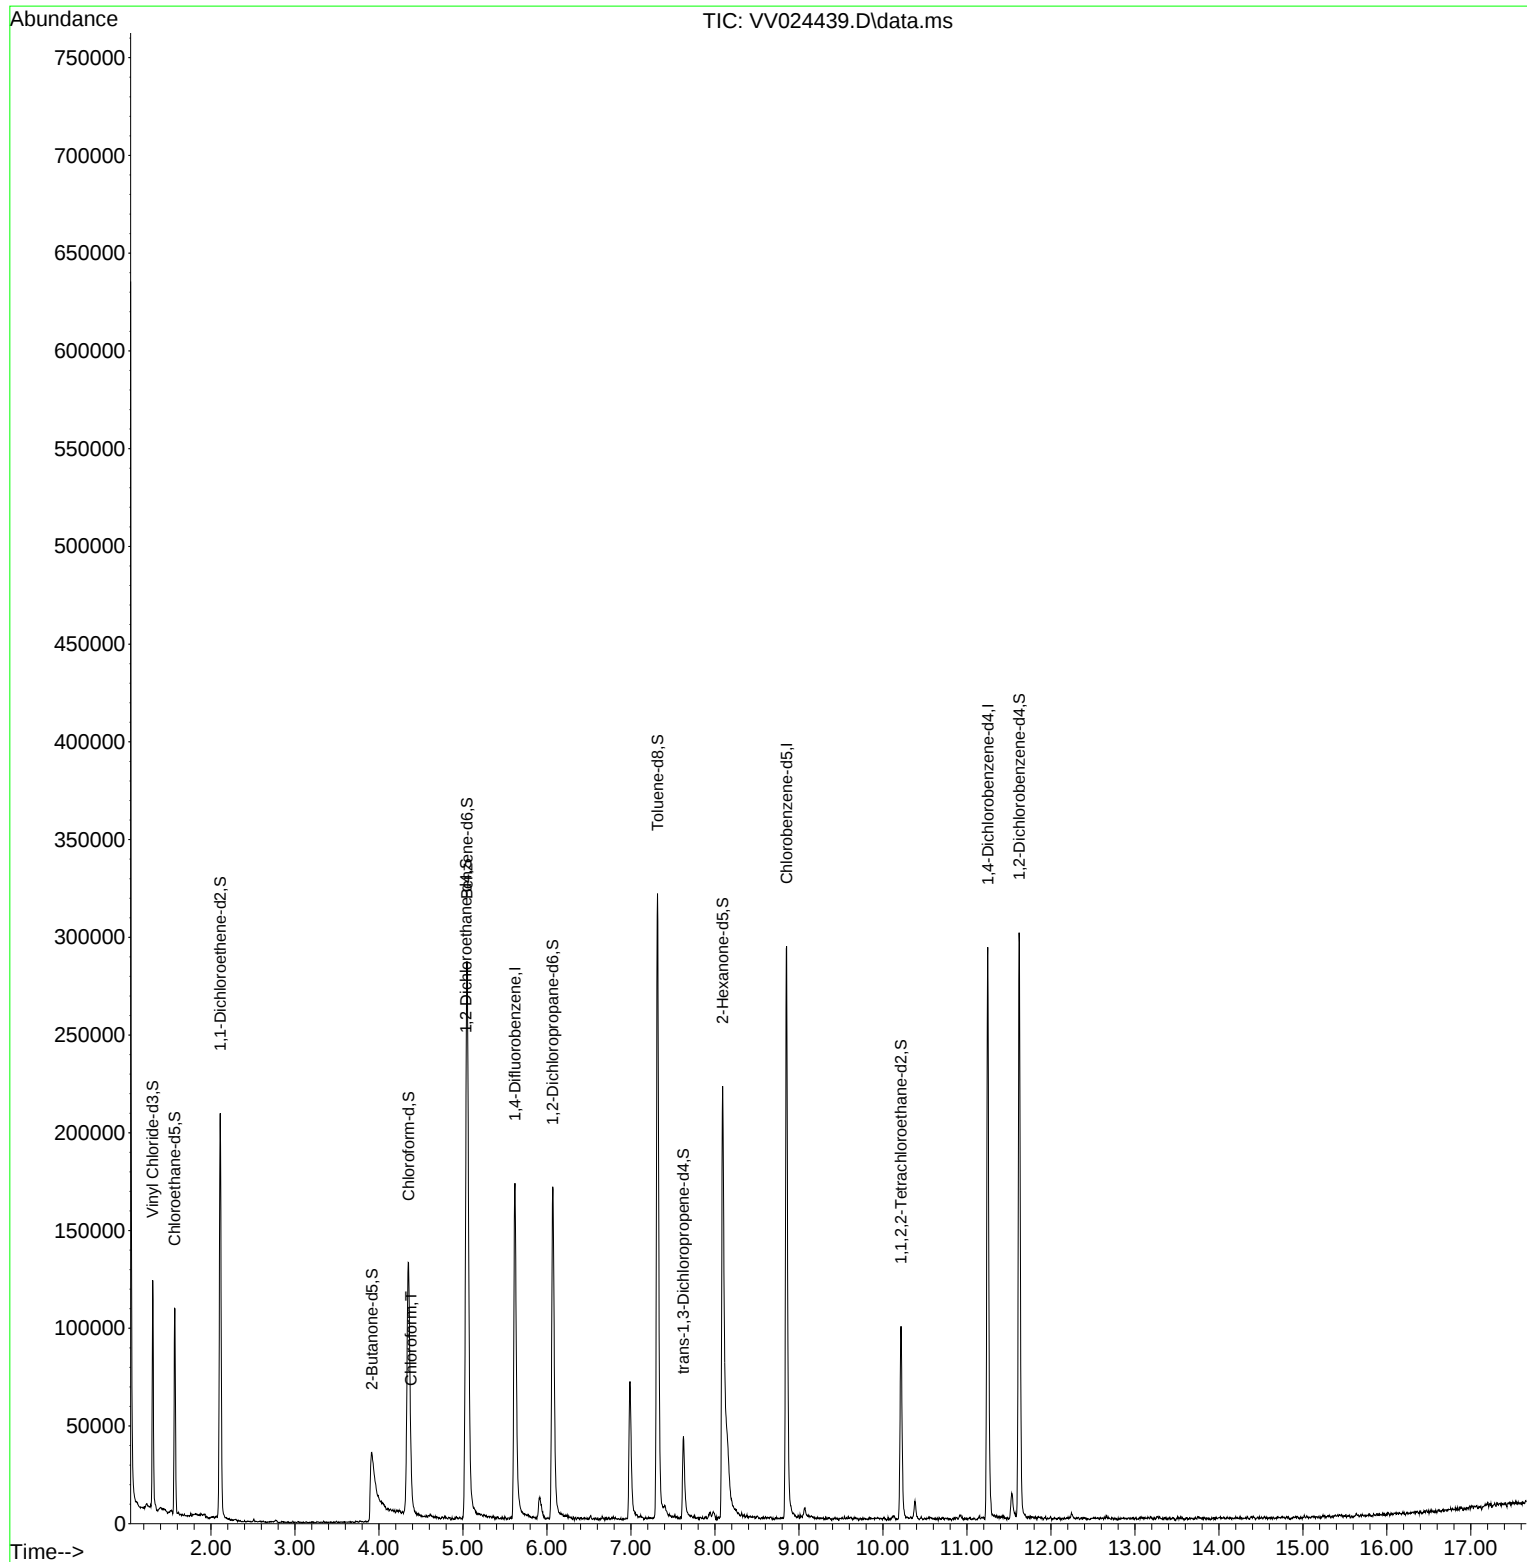

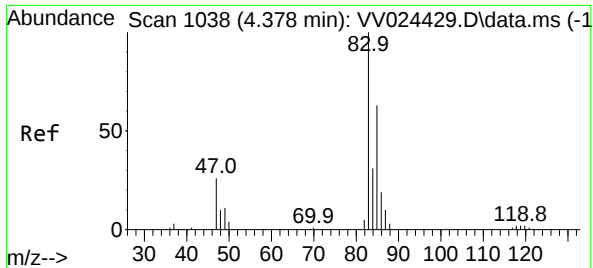

#25
Chloroform
Concen: 0.244 ug/L
RT: 4.381 min Scan# 10
Delta R.T. 0.003 min
Lab File: VV024439.D
Acq: 26 Jan 2022 15:14

Instrument :
MSVOA_V
ClientSampleId :
C0F28

Tgt Ion: 83 Resp: 5360
Ion Ratio Lower Upper
83 100
85 66.2 45.2 84.0

