

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW012622\
 Data File : VW024445.D
 Acq On : 26 Jan 2022 17:33
 Operator : SY/MD
 Sample : N1275-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F47

Quant Time: Jan 27 03:51:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 27 01:56:16 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	154939	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	168586	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	83650	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	67853	4.999	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 100.000%		
7) Chloroethane-d5	1.568	69	63032	5.323	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 106.400%		
11) 1,1-Dichloroethene-d2	2.108	63	104654	4.034	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 80.600%		
20) 2-Butanone-d5	3.905	46	94533	43.697	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	= 87.400%		
24) Chloroform-d	4.352	84	136558	5.302	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 106.000%		
26) 1,2-Dichloroethane-d4	5.034	65	63900	5.478	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 109.600%		
32) Benzene-d6	5.053	84	256427	5.093	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 101.800%		
36) 1,2-Dichloropropane-d6	6.069	67	82537	5.206	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 104.200%		
41) Toluene-d8	7.317	98	216171	4.679	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 93.600%		
43) trans-1,3-Dichloroprop...	7.625	79	24238	4.452	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 89.000%		
46) 2-Hexanone-d5	8.091	63	88494	47.537	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 95.080%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	48113	5.098	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 102.000%		
66) 1,2-Dichlorobenzene-d4	11.625	152	79948	5.574	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 111.400%		
Target Compounds						
25) Chloroform	4.381	83	9925	0.420	ug/L	99
34) Trichloroethene	5.924	95	4771	0.374	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV012622\
Data File : VV024445.D
Acq On : 26 Jan 2022 17:33
Operator : SY/MD
Sample : N1275-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F47

Quant Time: Jan 27 03:51:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 27 01:56:16 2022
Response via : Initial Calibration

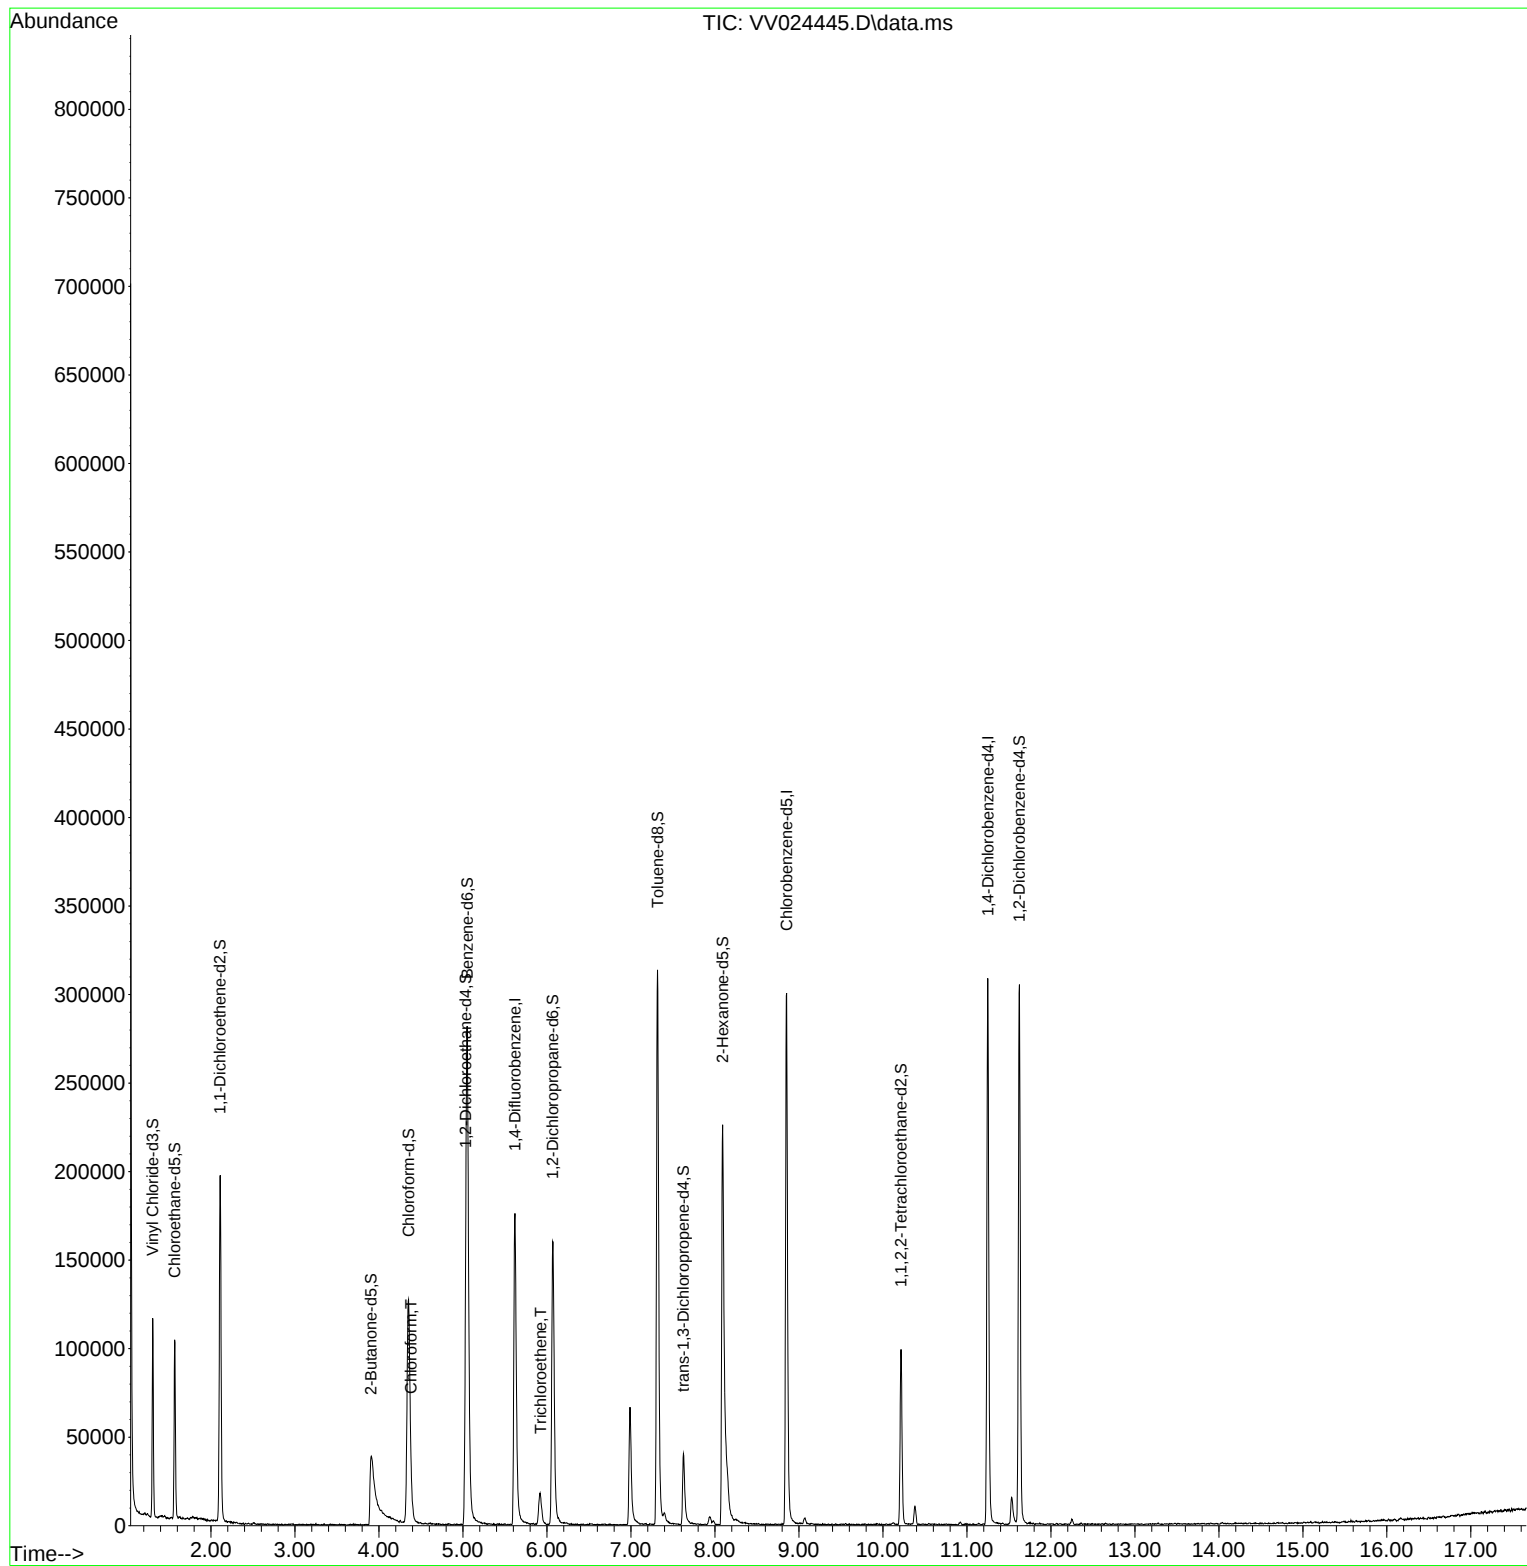

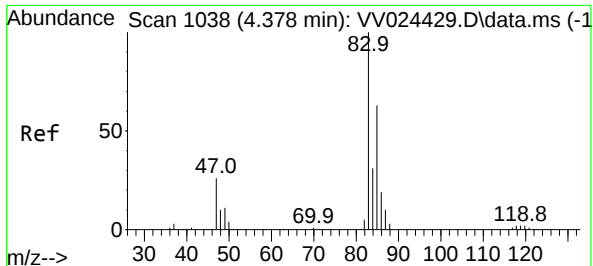

#25

Chloroform

Concen: 0.420 ug/L

RT: 4.381 min Scan# 1038

Delta R.T. 0.003 min

Lab File: VV024445.D

Acq: 26 Jan 2022 17:33

Instrument :

MSVOA_V

ClientSampleId :





C0F47

Tgt Ion: 83 Resp: 9925

Ion Ratio Lower Upper

83 100

85 65.3 45.2 84.0

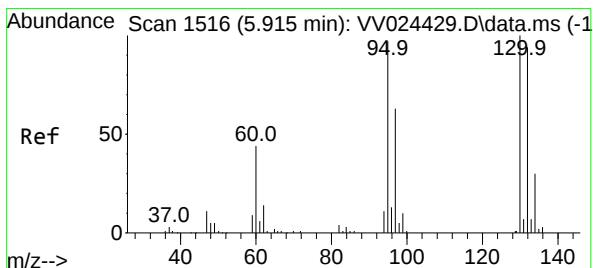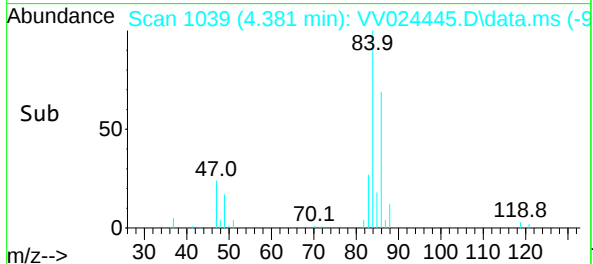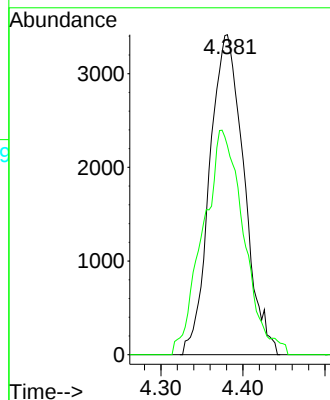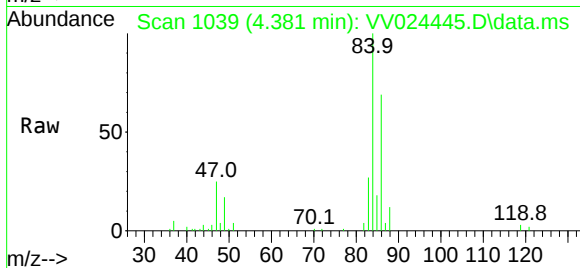

#34

Trichloroethene

Concen: 0.374 ug/L

RT: 5.924 min Scan# 1519

Delta R.T. 0.009 min

Lab File: VV024445.D

Acq: 26 Jan 2022 17:33

Tgt Ion: 95 Resp: 4771

Ion Ratio Lower Upper

95 100

97 72.9 45.2 84.0

132 94.5 76.1 141.3

130 108.3 75.4 140.0

